


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011019\
 Data File : BM018528.D
 Acq On : 11 Jan 2019 04:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

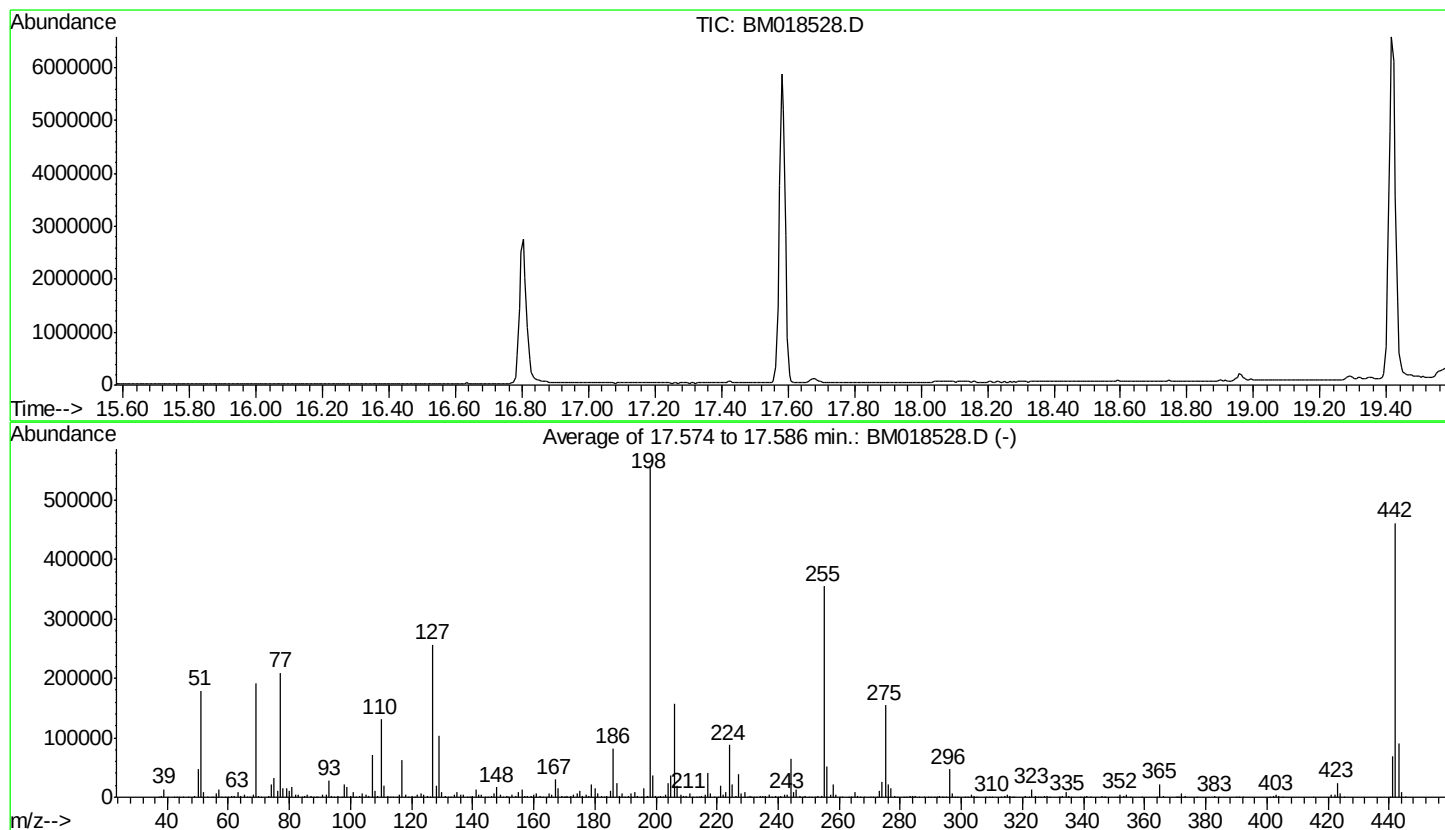

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	179221	PASS
68	69	0.00	2	1.9	3702	PASS
69	198	0.00	100	34.4	191882	PASS
70	69	0.00	2	0.8	1457	PASS
127	198	10	80	46.0	256512	PASS
197	198	0.00	2	0.4	2197	PASS
198	198	100	100	100.0	557781	PASS
199	198	5	9	6.7	37104	PASS
275	198	10	60	27.6	154149	PASS
365	198	1	100	3.9	21680	PASS
441	198	0.01	100	12.5	69560	PASS
442	198	50	100	82.7	461226	PASS
443	442	15	24	19.8	91544	PASS