

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011119\
 Data File : BM018544.D
 Acq On : 11 Jan 2019 20:57
 Operator : JU/SJ
 Sample : K1088-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB-1

Quant Time: Jan 12 00:11:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 10 05:57:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	329991	20.00	ng	0.00
21) Naphthalene-d8	10.55	136	1368500	20.00	ng	0.00
39) Acenaphthene-d10	14.40	164	821570	20.00	ng	0.00
64) Phenanthrene-d10	17.15	188	2005871	20.00	ng	0.00
76) Chrysene-d12	21.34	240	2518156	20.00	ng	0.00
87) Perylene-d12	23.63	264	2958754	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	1119055	62.62	ng	0.00
7) Phenol-d6	6.93	99	884283	38.96	ng	0.00
23) Nitrobenzene-d5	8.92	82	2097825	88.87	ng	0.00
42) 2,4,6-Tribromophenol	15.90	330	1657419	158.44	ng	0.00
45) 2-Fluorobiphenyl	13.02	172	5381596	85.47	ng	0.00
79) Terphenyl-d14	19.79	244	10320570	86.40	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011119\
Data File : BM018544.D
Acq On : 11 Jan 2019 20:57
Operator : JU/SJ
Sample : K1088-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-1

Quant Time: Jan 12 00:11:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

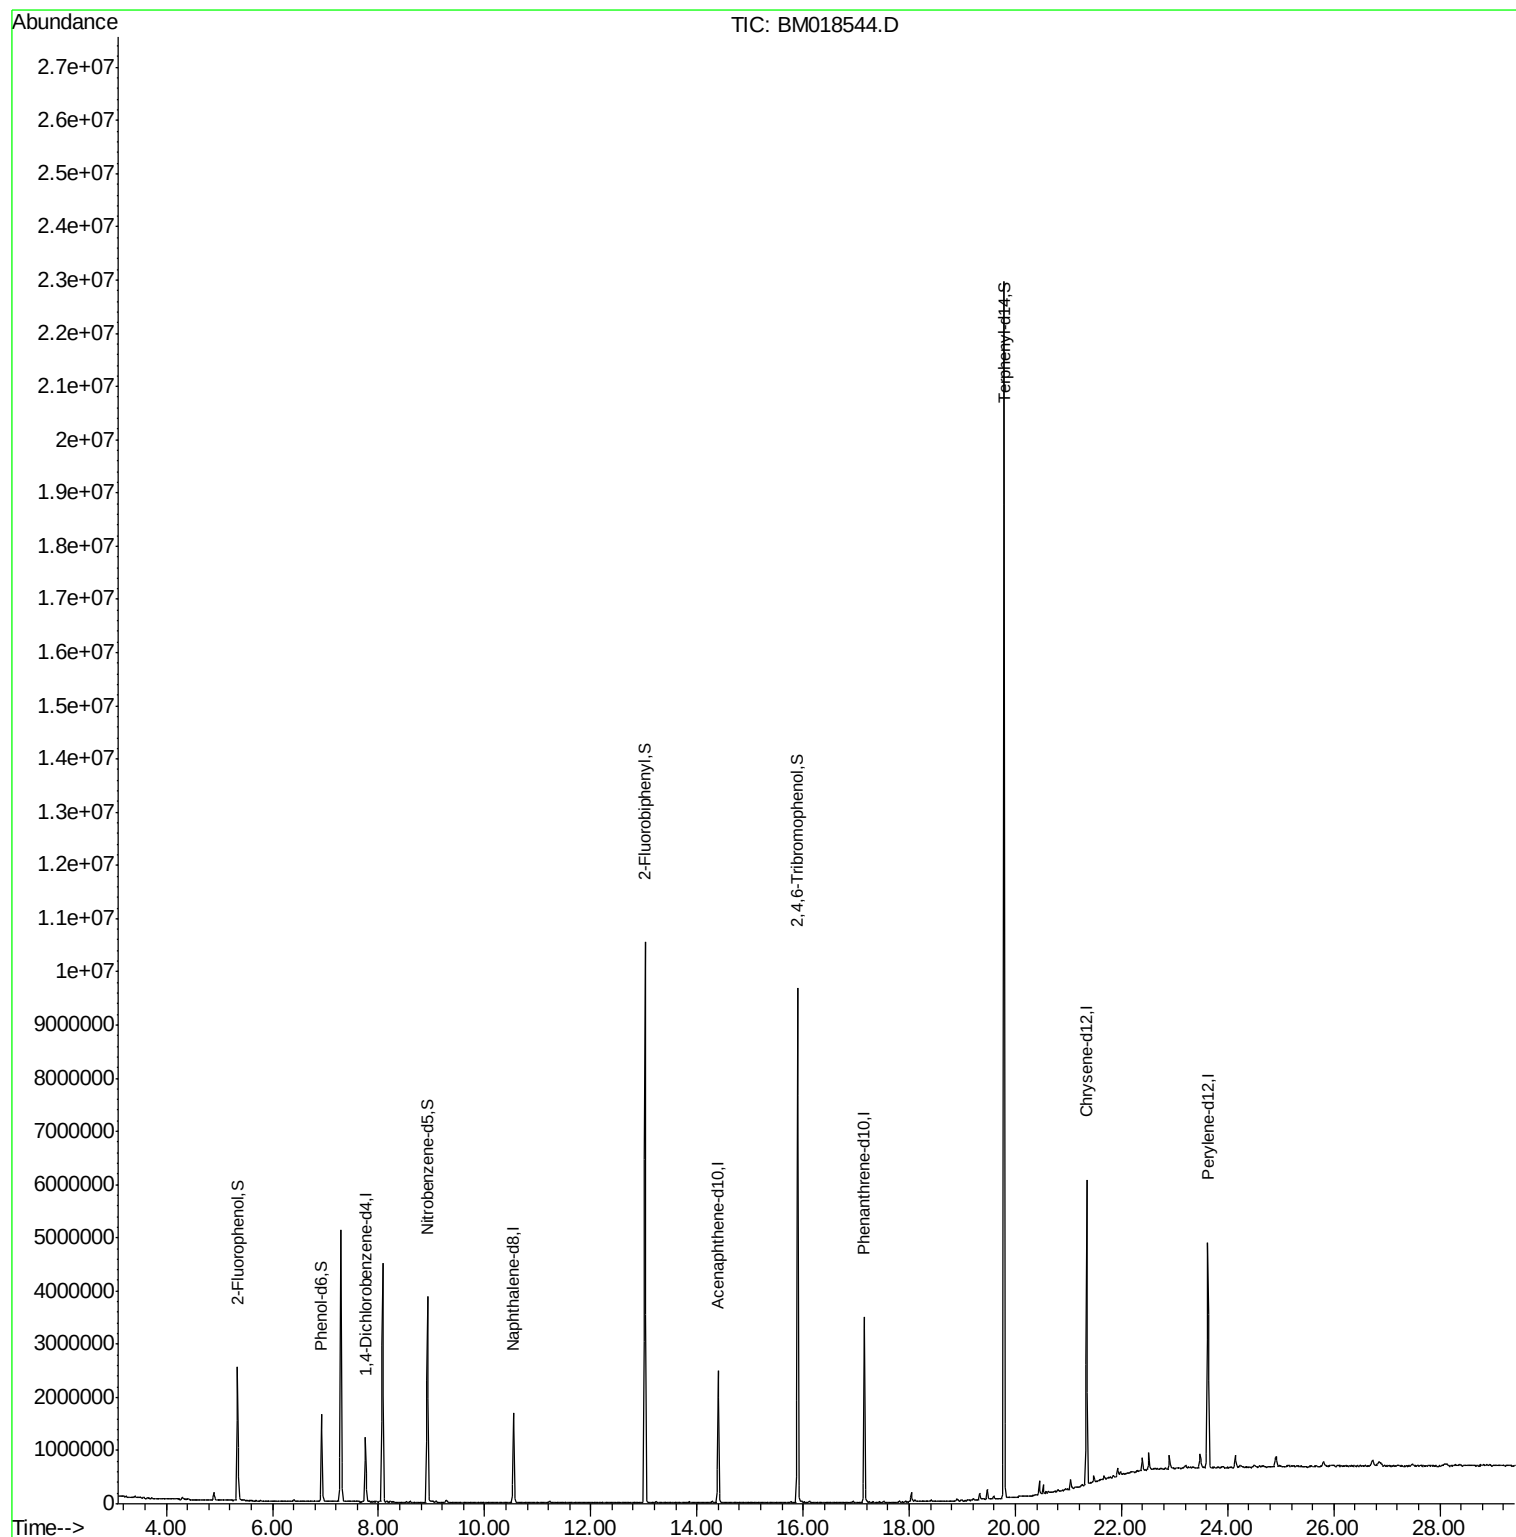

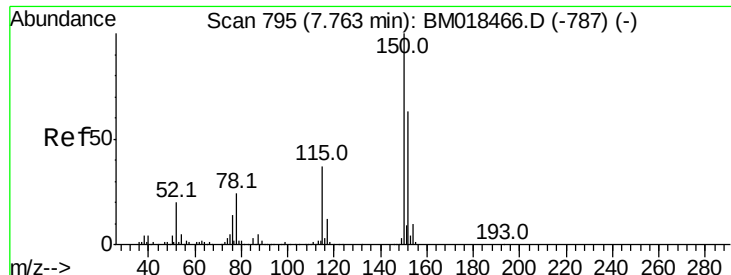


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.76 min Scan# 794
Delta R.T. -0.01 min
Lab File: BM018544.D
Acq: 11 Jan 2019 20:57

Instrument :
BNA_M
ClientSampled :
FB-1

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.7	126.9	190.3
115	59.1	45.5	68.3



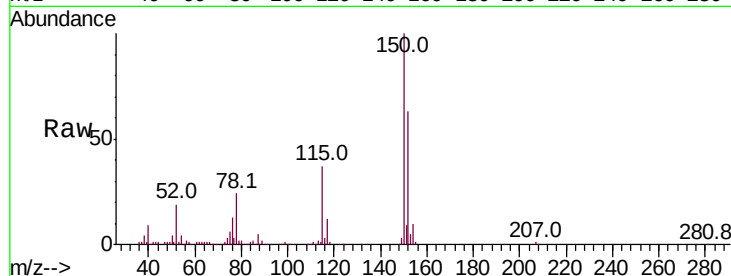


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

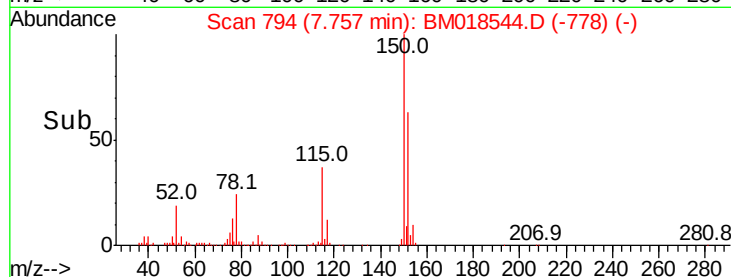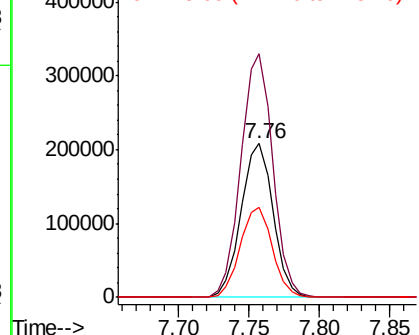

#5

2-Fluorophenol
Concen: 62.618 ng
RT: 5.35 min Scan# 384
Delta R.T. -0.01 min
Lab File: BM018544.D
Acq: 11 Jan 2019 20:57

Tgt Ion	Ratio	Lower	Upper
112	100		
64	52.6	46.5	69.7
63	29.6	25.2	37.8






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

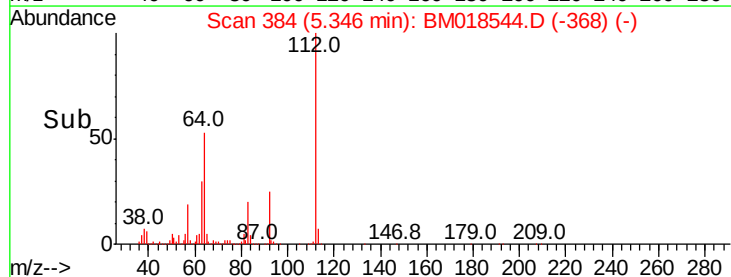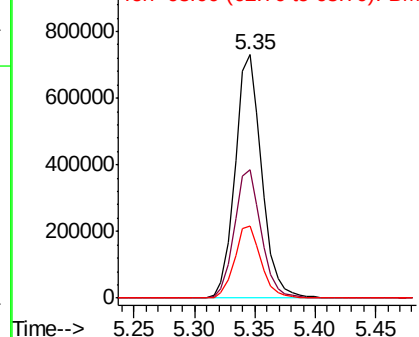

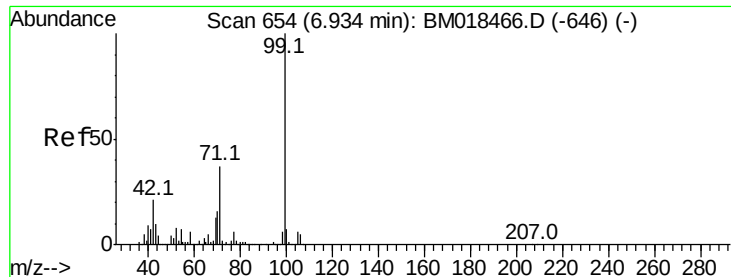

#7

Phenol-d6

Concen: 38.958 ng

RT: 6.93 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM018544.D

Acq: 11 Jan 2019 20:57

Instrument :

BNA_M

ClientSampleId :

FB-1


Tot Ion: 99 Resp: 884283

Ion Ratio Lower Upper

99 100

42 20.0 17.3 25.9




71 36.3 28.0 42.0

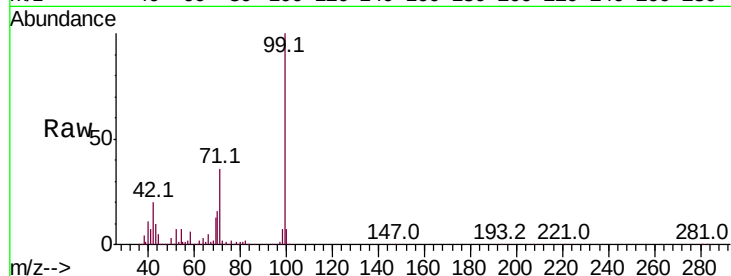

Abundance Ion 99.00 (98.70 to 99.70): BM018466.D (-646) (-)

Ion 42.00 (41.70 to 42.70): BM018466.D (-646) (-)

Ion 71.00 (70.70 to 71.70): BM018466.D (-646) (-)

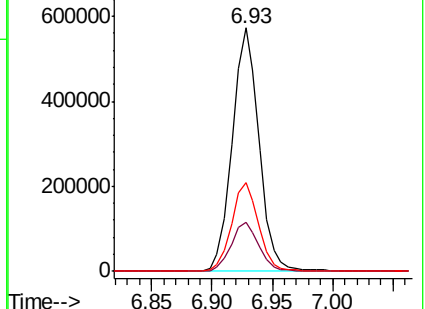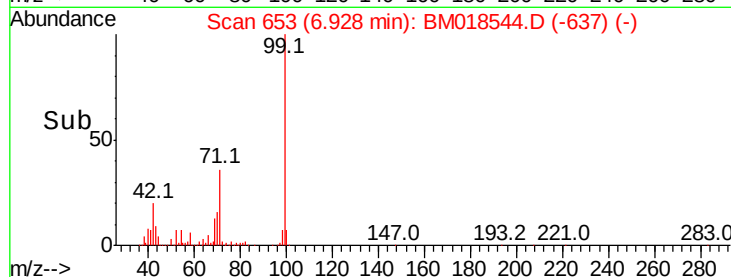

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.55 min Scan# 1268

Delta R.T. -0.01 min

Lab File: BM018544.D

Acq: 11 Jan 2019 20:57

Tgt Ion: 136 Resp: 1368500


Ion Ratio Lower Upper

136 100

137 10.6 8.5 12.7

54 6.3 6.0 9.0

68 4.5 4.5 6.7






Abundance Ion 136.00 (135.70 to 136.70): BM018466.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM018466.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM018466.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM018466.D (-1261) (-)



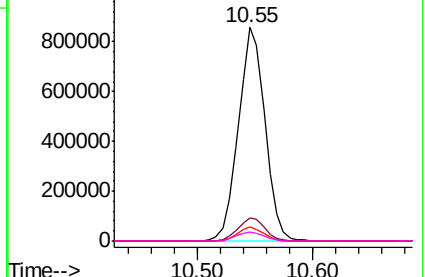
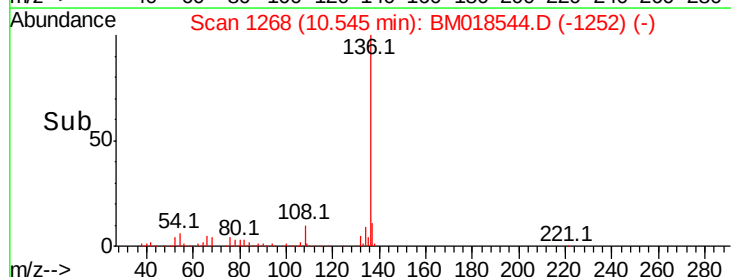


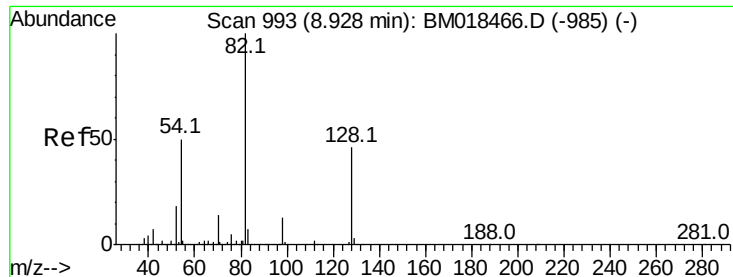

#23
Nitrobenzene-d5
Concen: 88.866 ng
RT: 8.92 min Scan# 992
Delta R.T. -0.00 min
Lab File: BM018544.D
Acq: 11 Jan 2019 20:57




Instrument :
BNA_M
ClientSampleId :
FB-1


Tot Ion: 82 Resp: 2097825
Ion Ratio Lower Upper
82 100
128 46.7 36.3 54.5
54 49.2 41.7 62.5

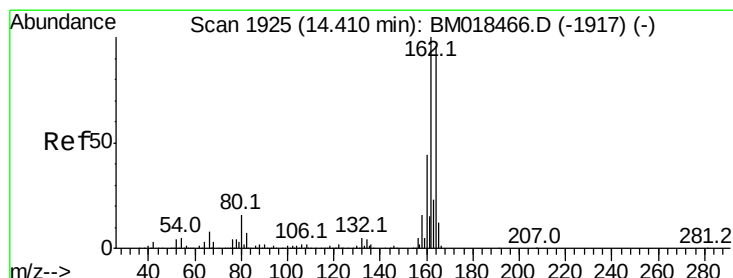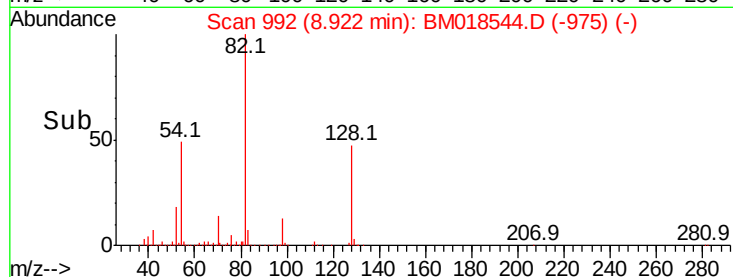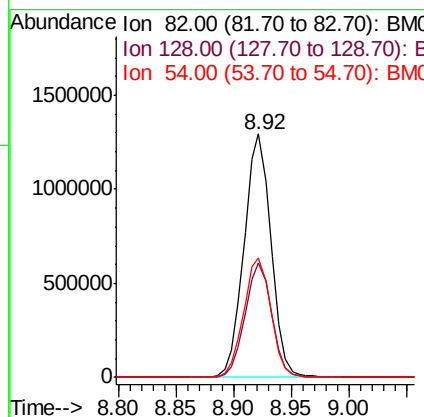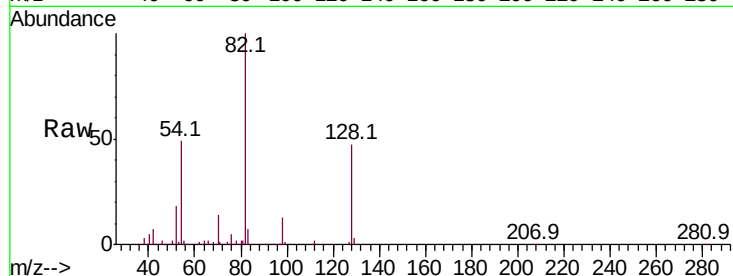

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.40 min Scan# 1924
Delta R.T. -0.01 min
Lab File: BM018544.D
Acq: 11 Jan 2019 20:57

Tgt Ion: 164 Resp: 821570
Ion Ratio Lower Upper
164 100
162 102.8 83.0 124.4
160 46.1 37.1 55.7

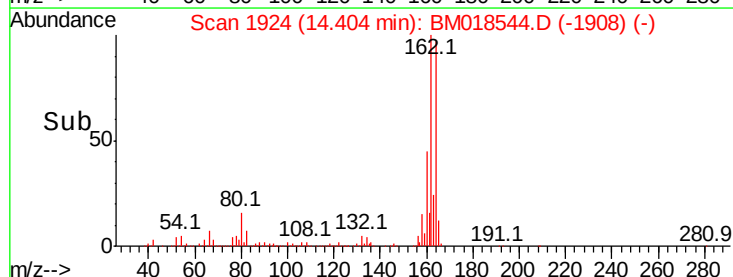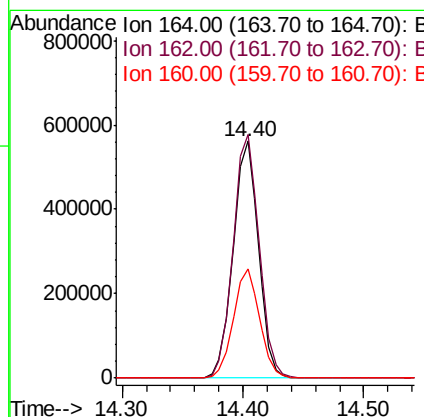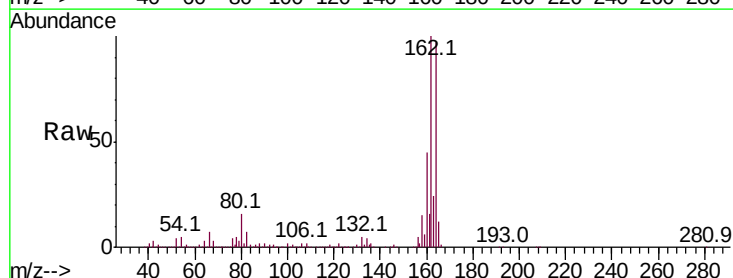

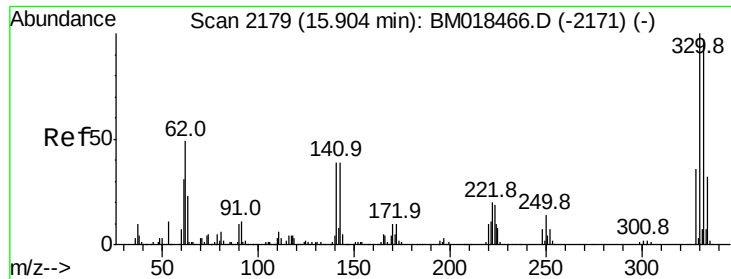


#42
 2,4,6-Tribromophenol
 Concen: 158.440 ng
 RT: 15.90 min Scan# 2178
 Delta R.T. -0.01 min
 Lab File: BM018544.D
 Acq: 11 Jan 2019 20:57




Instrument :
 BNA_M
 ClientSampled :
 FB-1

Tot Ion:330 Resp: 1657419

Ion	Ratio	Lower	Upper
330	100		
332	97.3	77.6	116.4
141	38.8	31.7	47.5




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

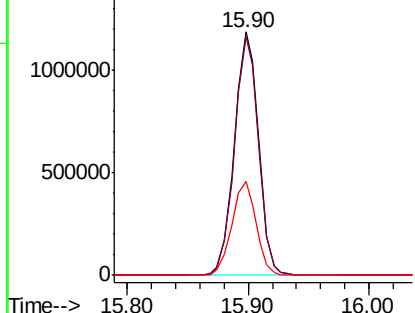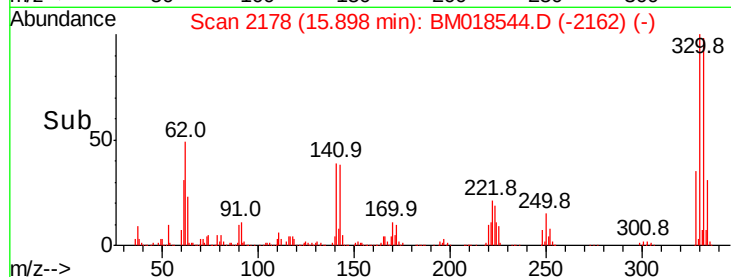



#45
 2-Fluorobiphenyl
 Concen: 85.473 ng
 RT: 13.02 min Scan# 1689
 Delta R.T. -0.00 min
 Lab File: BM018544.D
 Acq: 11 Jan 2019 20:57


Tgt Ion:172 Resp: 5381596

Ion	Ratio	Lower	Upper
172	100		
171	35.3	28.2	42.4
170	23.3	18.9	28.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

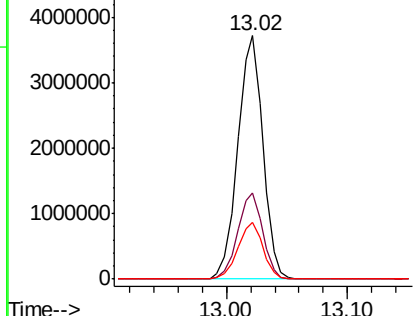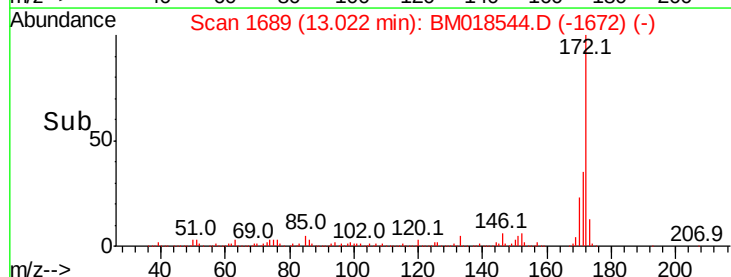

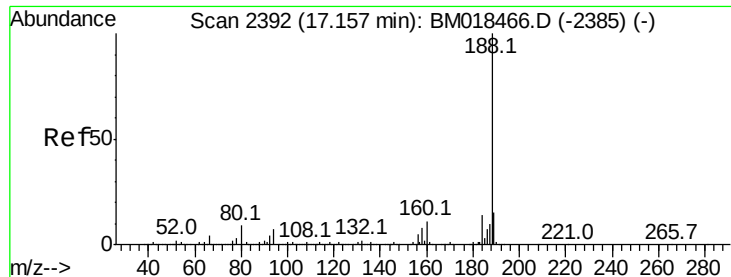

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.15 min Scan# 2391

Delta R.T. -0.01 min

Lab File: BM018544.D

Acq: 11 Jan 2019 20:57

Instrument :

BNA_M

ClientSampleId :

FB-1


Tot Ion:188 Resp: 2005871

Ion Ratio Lower Upper

188 100

94 7.6 7.1 10.7




80 8.3 7.6 11.4



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

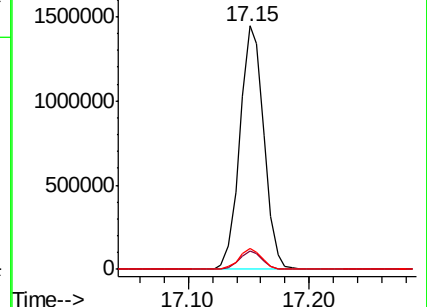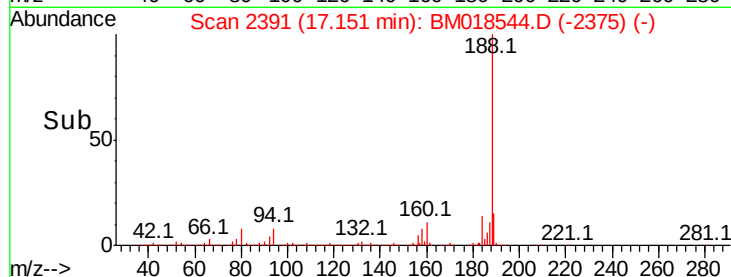

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.34 min Scan# 3104

Delta R.T. -0.01 min

Lab File: BM018544.D

Acq: 11 Jan 2019 20:57


Tgt Ion:240 Resp: 2518156

Ion Ratio Lower Upper

240 100

120 9.3 8.4 12.6



236 25.8 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

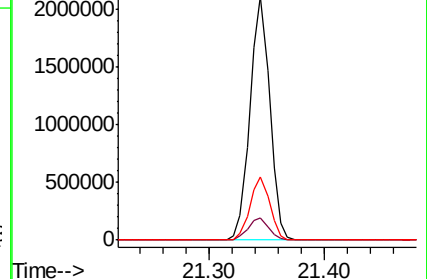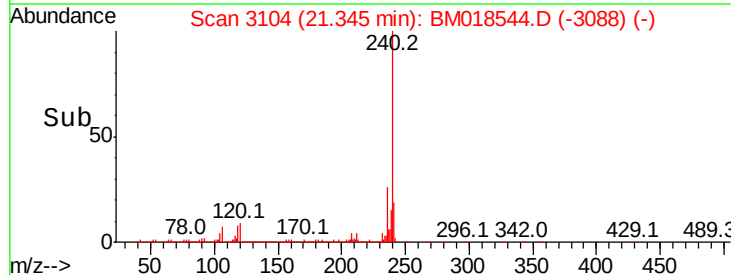




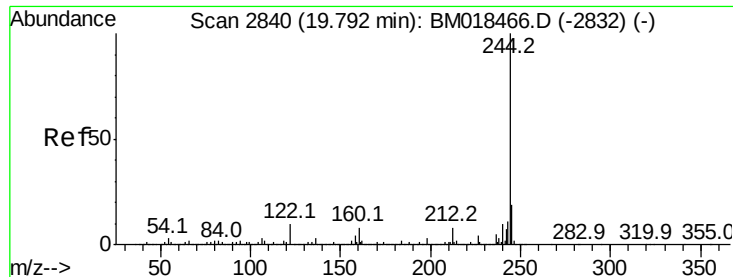


#79
 Terphenyl-d14
 Concen: 86.397 ng
 RT: 19.79 min Scan# 2839
 Delta R.T. -0.00 min
 Lab File: BM018544.D
 Acq: 11 Jan 2019 20:57

Instrument :
 BNA_M
 ClientSampled :
 FB-1

Tot Ion:244 Resp:10320570

Ion	Ratio	Lower	Upper
244	100		
212	7.9	5.9	8.9
122	9.8	9.0	13.4

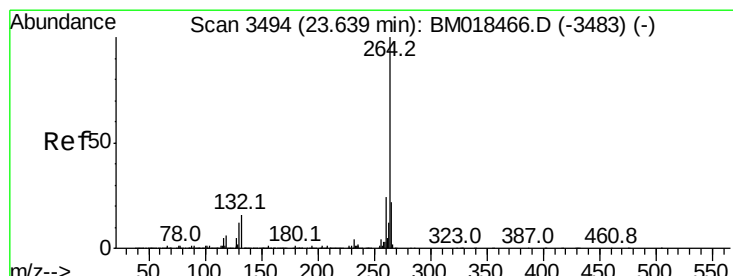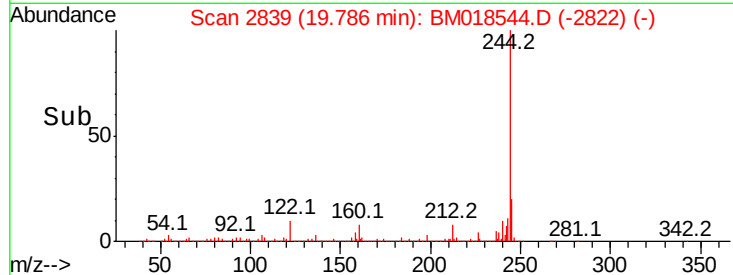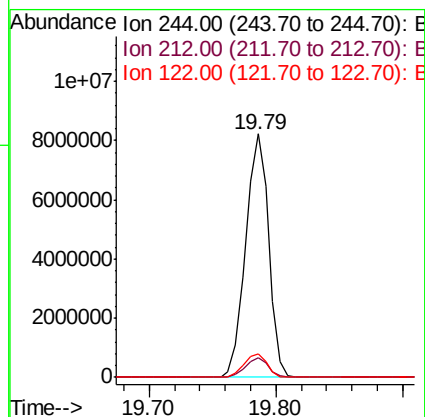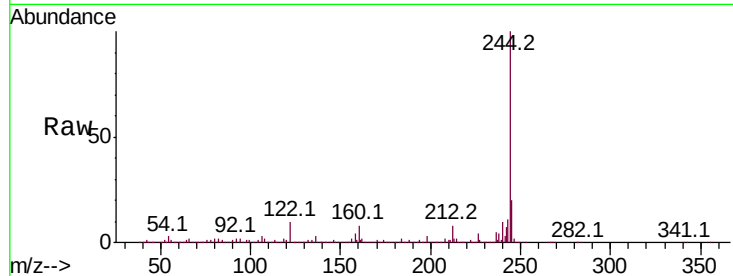

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.63 min Scan# 3492
 Delta R.T. -0.01 min
 Lab File: BM018544.D
 Acq: 11 Jan 2019 20:57

Tgt Ion:264 Resp: 2958754

Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.9	28.3
265	22.0	16.8	25.2

