
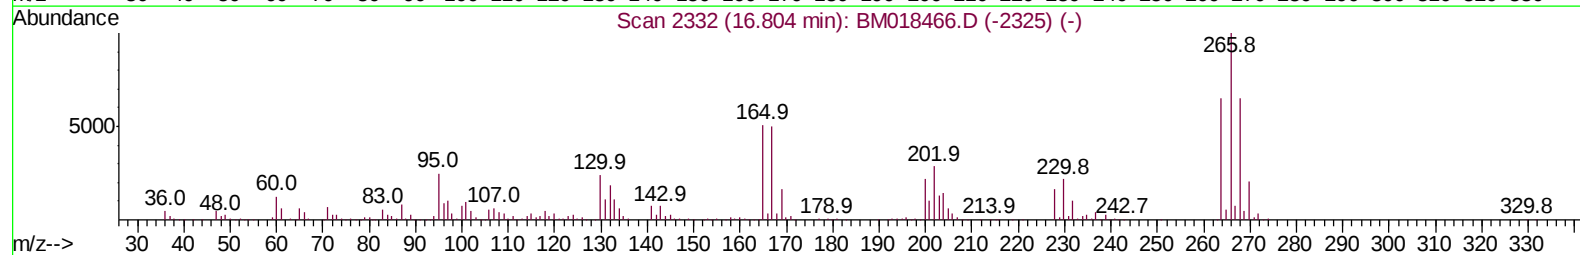
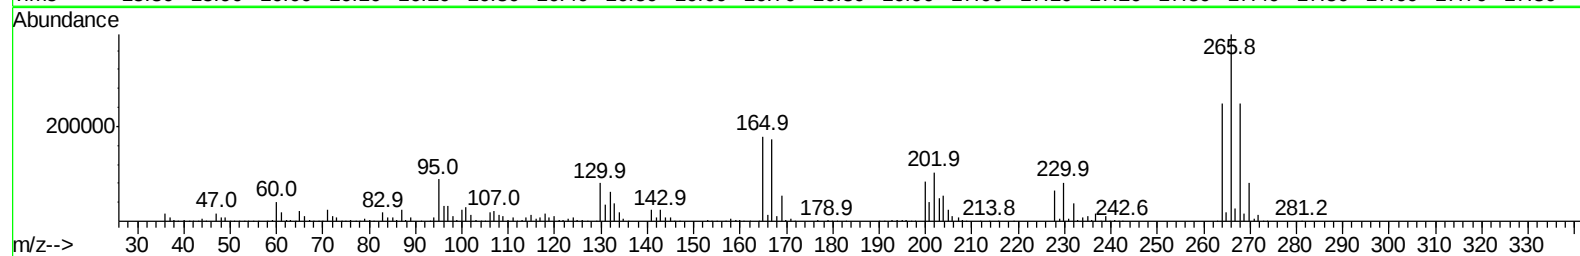


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011119\
Data File : BM018535.D
Acq On : 11 Jan 2019 12:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 01:35:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

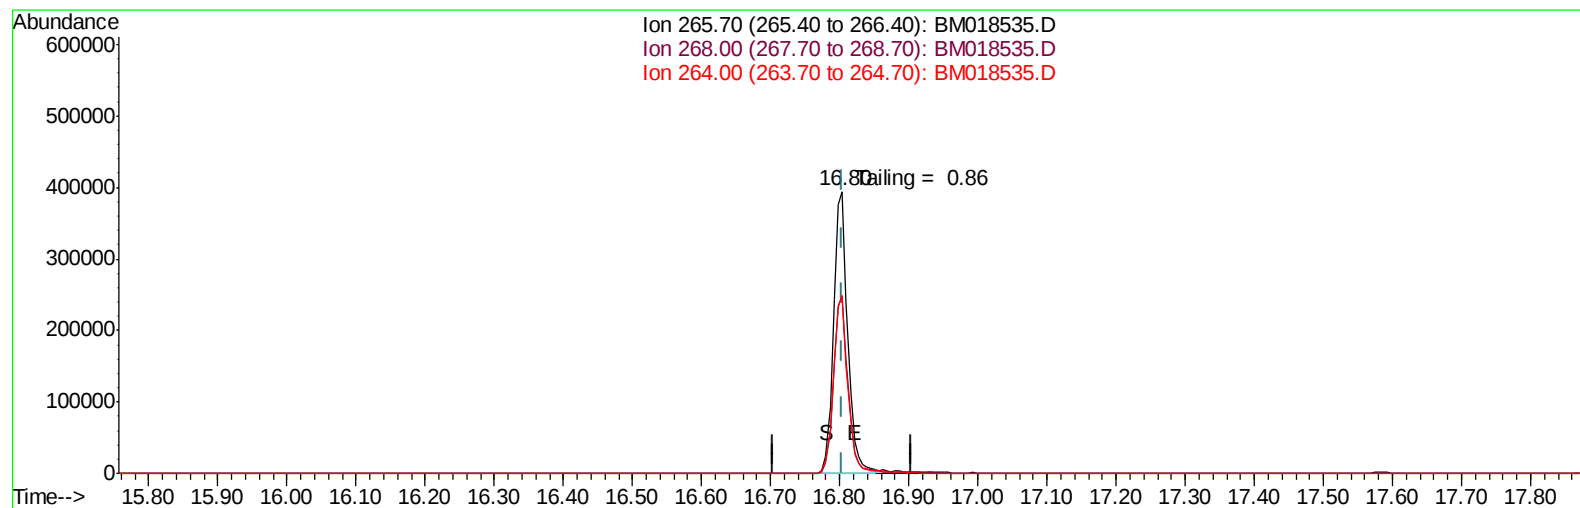

TIC: BM018535.D

(70) Pentachlorophenol (C)




16.804min (+0.000) 0.00ng

response 566196

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.77
264.00	62.60	63.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011119\
 Data File : BM018535.D
 Acq On : 11 Jan 2019 12:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 01:35:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 10 05:57:41 2019
 Response via : Initial Calibration

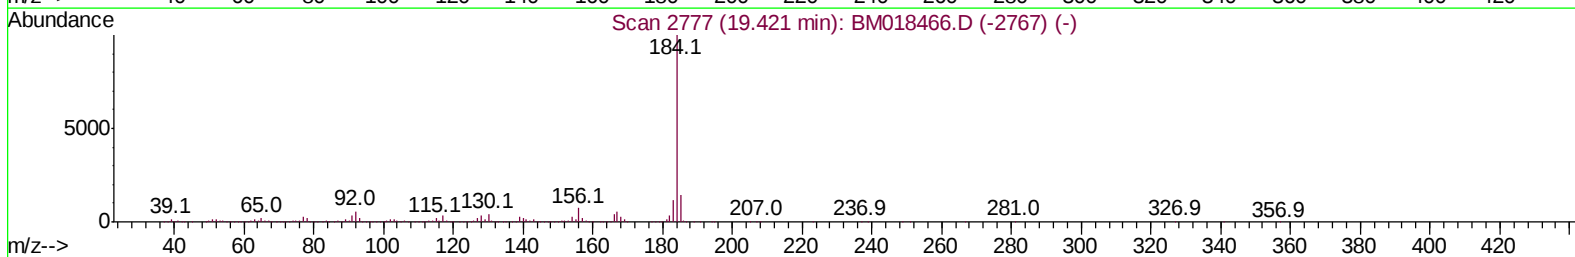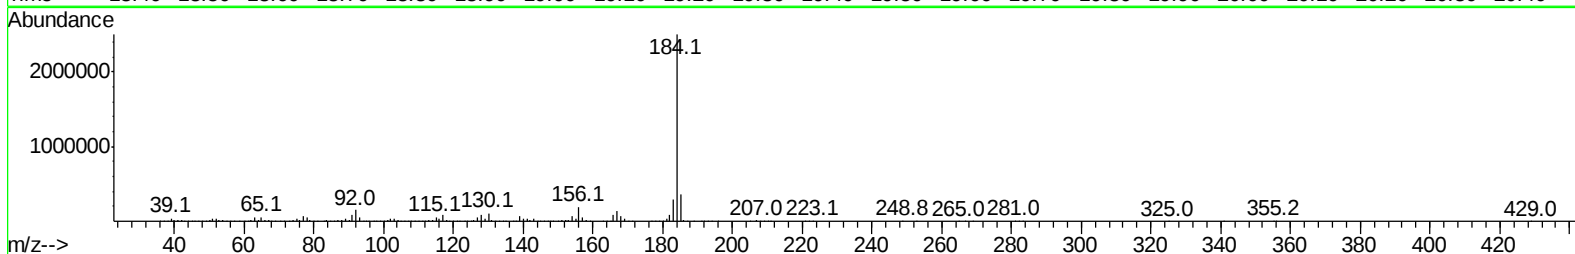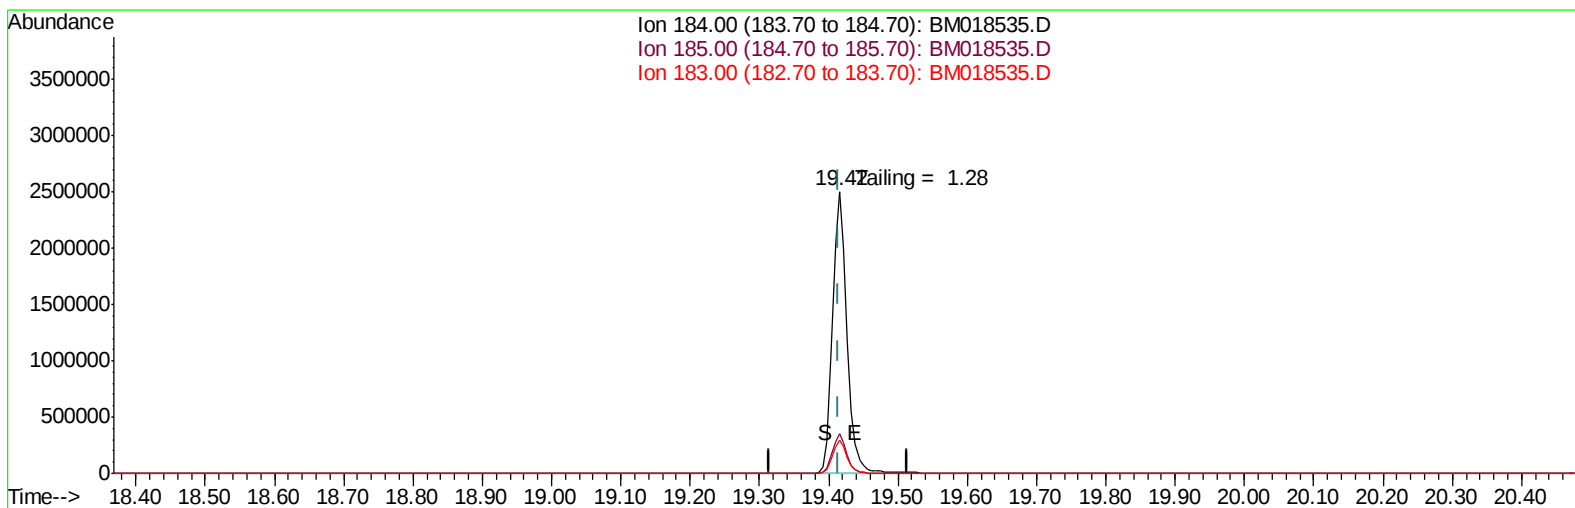

TIC: BM018535.D

(77) Benzidine

19.415min (-0.000) 515815.65ng

response 3591620

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.24
183.00	11.90	11.69
0.00	0.00	0.00