


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011119\
 Data File : BM018535.D
 Acq On : 11 Jan 2019 12:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

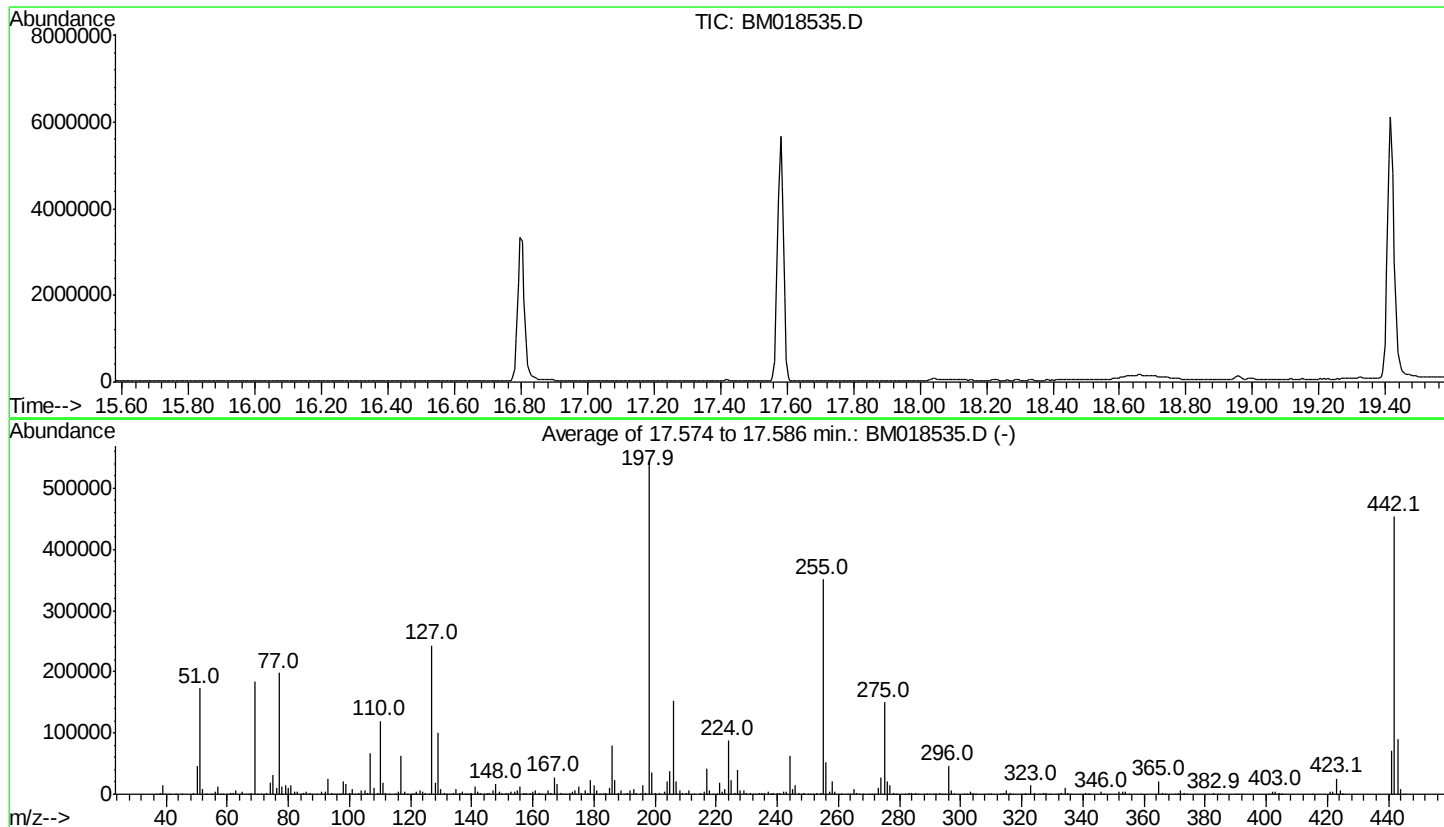

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	172821	PASS
68	69	0.00	2	1.6	2926	PASS
69	198	0.00	100	33.8	183151	PASS
70	69	0.00	2	0.2	351	PASS
127	198	10	80	45.0	243669	PASS
197	198	0.00	2	0.4	2077	PASS
198	198	100	100	100.0	541653	PASS
199	198	5	9	6.6	35730	PASS
275	198	10	60	27.8	150552	PASS
365	198	1	100	4.0	21928	PASS
441	198	0.01	100	13.0	70661	PASS
442	198	50	100	83.7	453354	PASS
443	442	15	24	19.8	89733	PASS