
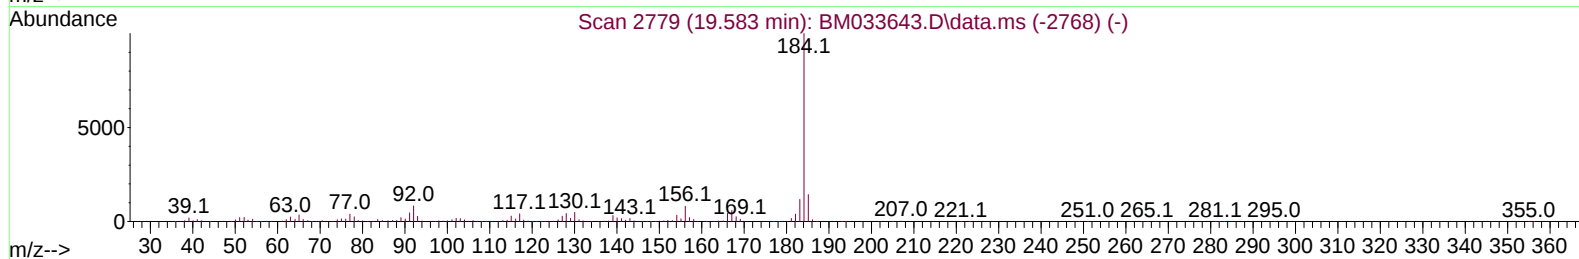
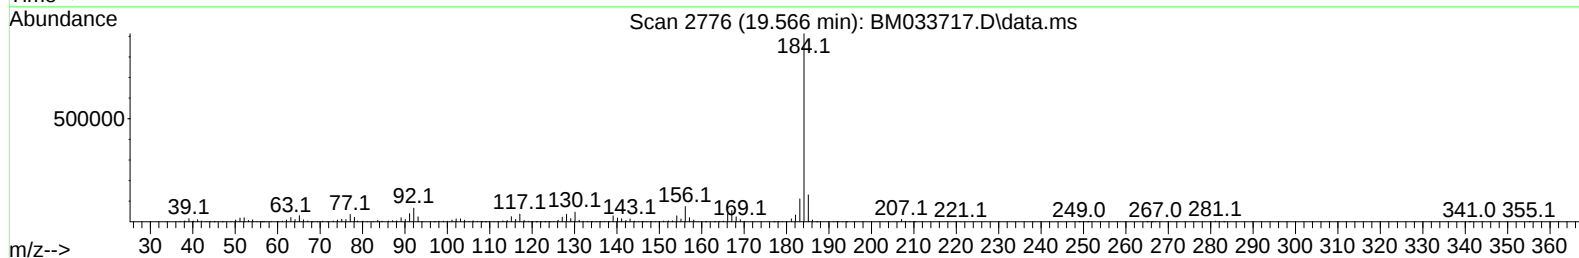


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011322\
 Data File : BM033717.D
 Acq On : 13 Jan 2022 15:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 21:31:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 13 07:49:01 2022
 Response via : Initial Calibration

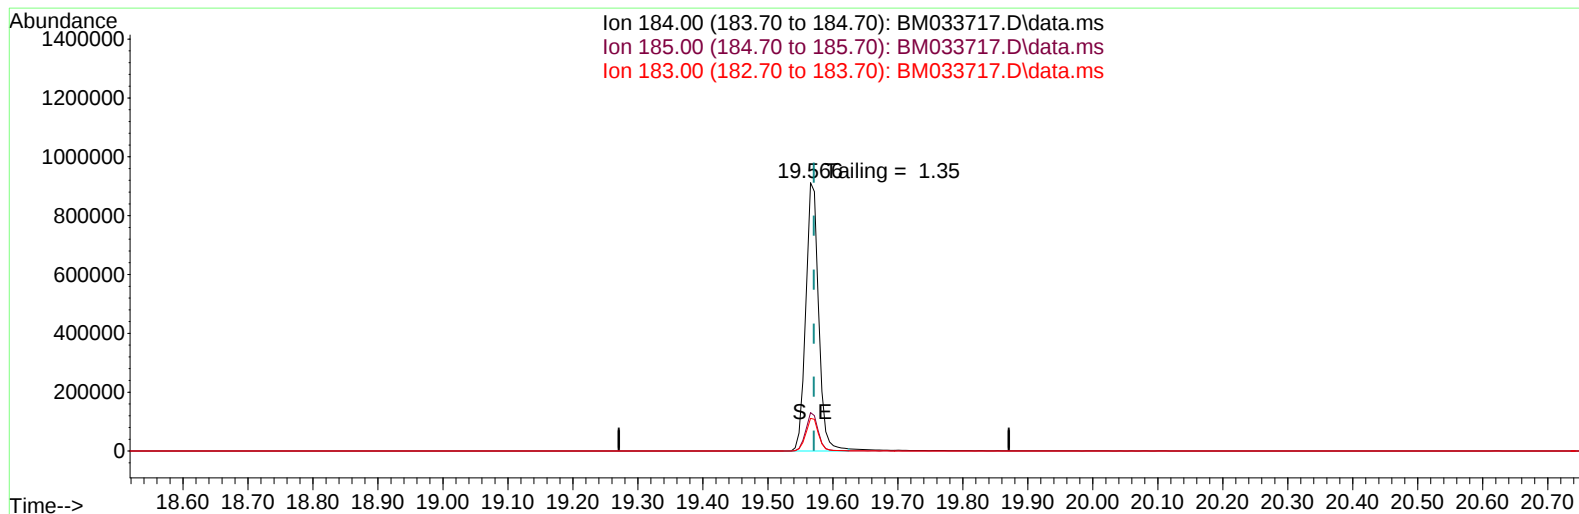




TIC: BM033717.D\data.ms

(77) Benzidine**19.566min (-0.005) 101836.00 ng****response 1274517**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.31
183.00	12.10	12.19
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011322\  
Data File : BM033717.D  
Acq On    : 13 Jan 2022  15:40  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jan 13 21:31:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 13 07:49:01 2022
Response via : Initial Calibration

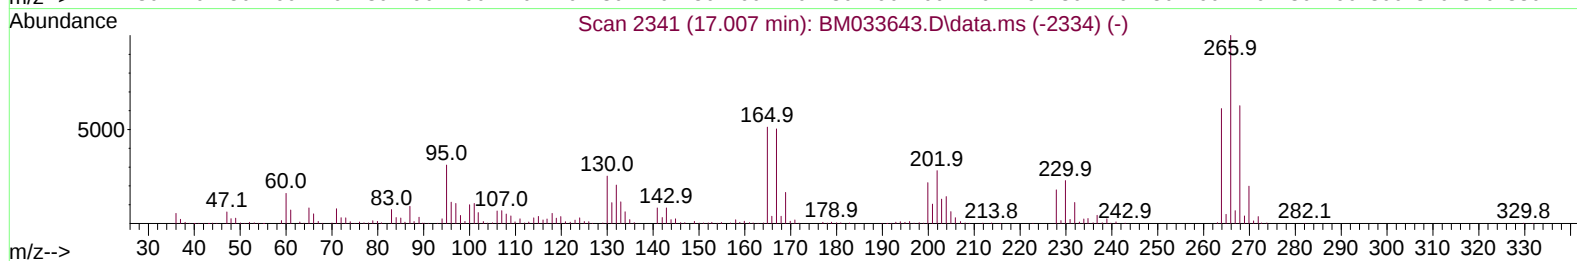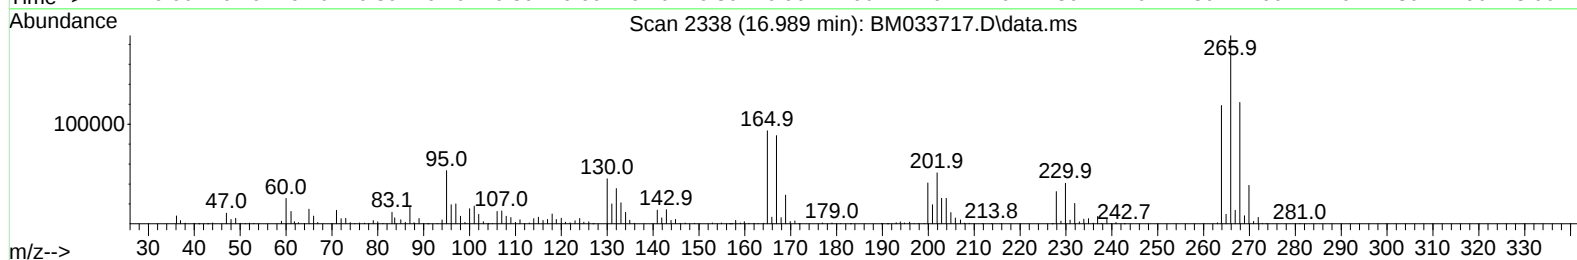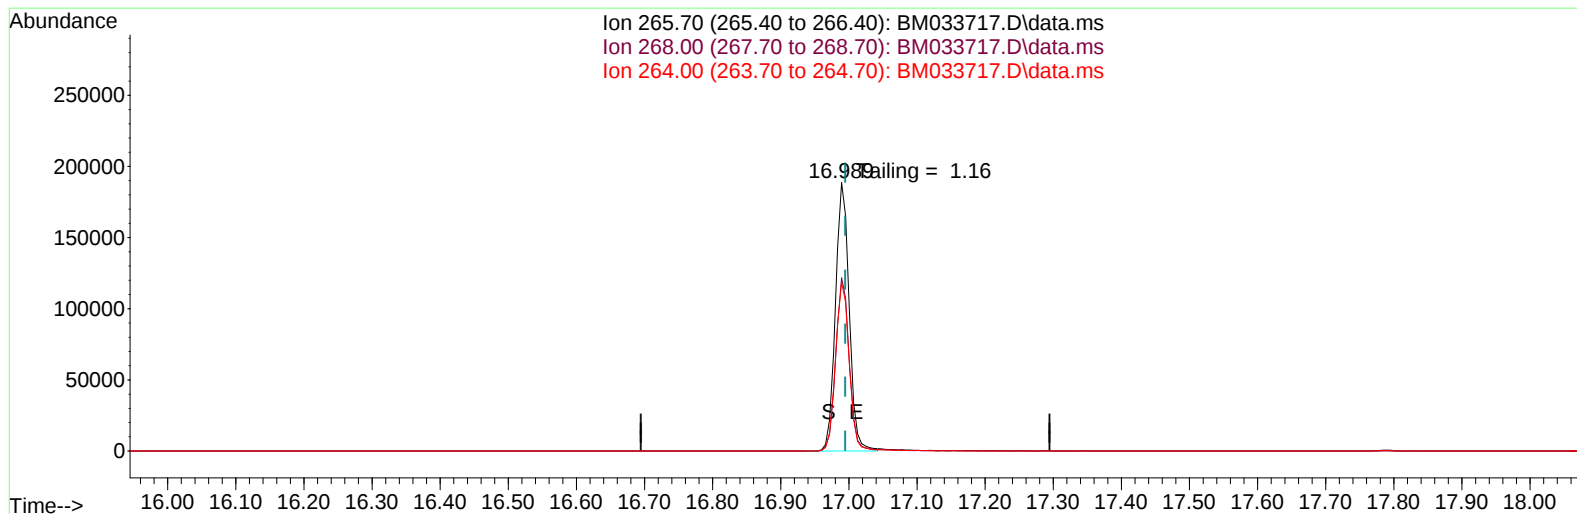

TIC: BM033717.D\data.ms

(70) Pentachlorophenol (C)

16.989min (-0.005) 0.00 ng

response **266116**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.55
264.00	61.40	62.90
0.00	0.00	0.00