

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011322\  
 Data File : BM033713.D  
 Acq On : 13 Jan 2022 12:01  
 Operator : CG/JU  
 Sample : PB141980BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB141980BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM010522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033713.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.513       | 380           | 387         | 396          | rBV      | 3246275        | 4620063       | 70.14%          | 12.327%       |
| 2         | 7.125       | 653           | 661         | 672          | rBV      | 2979117        | 4707655       | 71.47%          | 12.561%       |
| 3         | 7.966       | 797           | 804         | 811          | rBV      | 624898         | 972830        | 14.77%          | 2.596%        |
| 4         | 9.131       | 993           | 1002        | 1013         | rBV      | 1957660        | 3182082       | 48.31%          | 8.490%        |
| 5         | 10.784      | 1274          | 1283        | 1291         | rBV      | 791284         | 1351215       | 20.51%          | 3.605%        |
| 6         | 13.236      | 1692          | 1700        | 1715         | rBV      | 4606579        | 6586762       | 100.00%         | 17.574%       |
| 7         | 14.607      | 1926          | 1933        | 1944         | rBV      | 1026486        | 1529799       | 23.23%          | 4.082%        |
| 8         | 16.083      | 2178          | 2184        | 2199         | rBV      | 2389493        | 3500327       | 53.14%          | 9.339%        |
| 9         | 17.342      | 2391          | 2398        | 2408         | rBV      | 935084         | 1328356       | 20.17%          | 3.544%        |
| 10        | 19.953      | 2836          | 2842        | 2850         | rBV      | 5260125        | 6238612       | 94.71%          | 16.646%       |
| 11        | 21.500      | 3101          | 3105        | 3114         | rBV      | 1286137        | 1662345       | 25.24%          | 4.435%        |
| 12        | 23.924      | 3511          | 3517        | 3527         | rVB2     | 898868         | 1799049       | 27.31%          | 4.800%        |




Sum of corrected areas: 37479095

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011322\  
Data File : BM033713.D  
Acq On : 13 Jan 2022 12:01  
Operator : CG/JU  
Sample : PB141980BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB141980BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM010522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

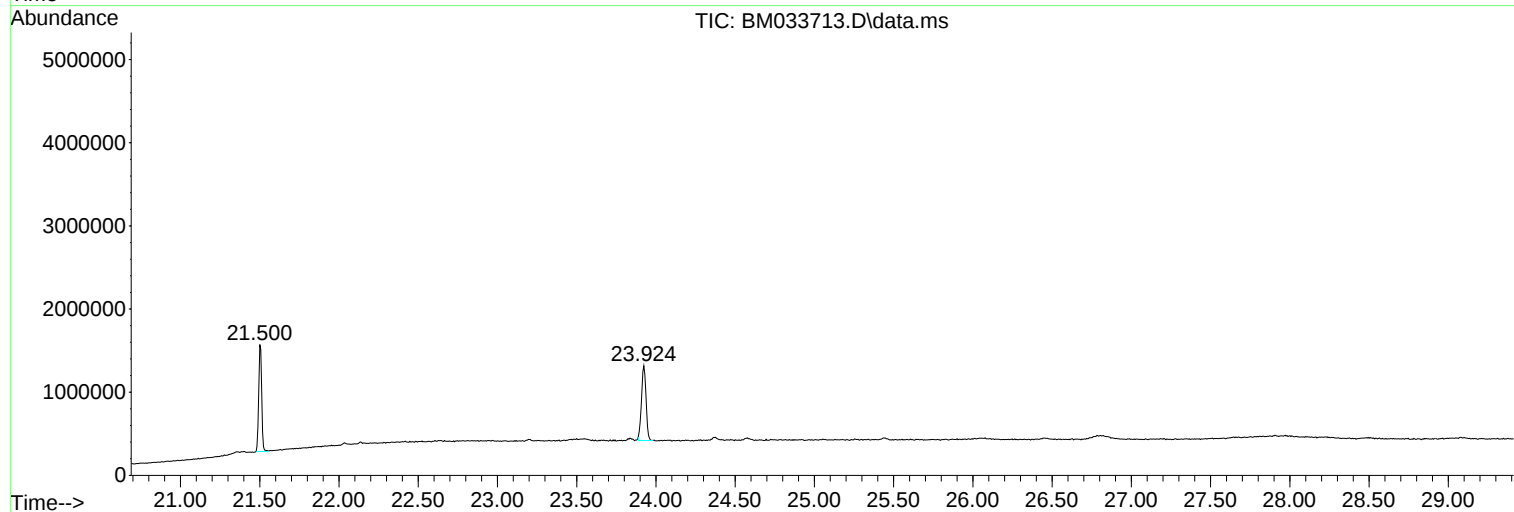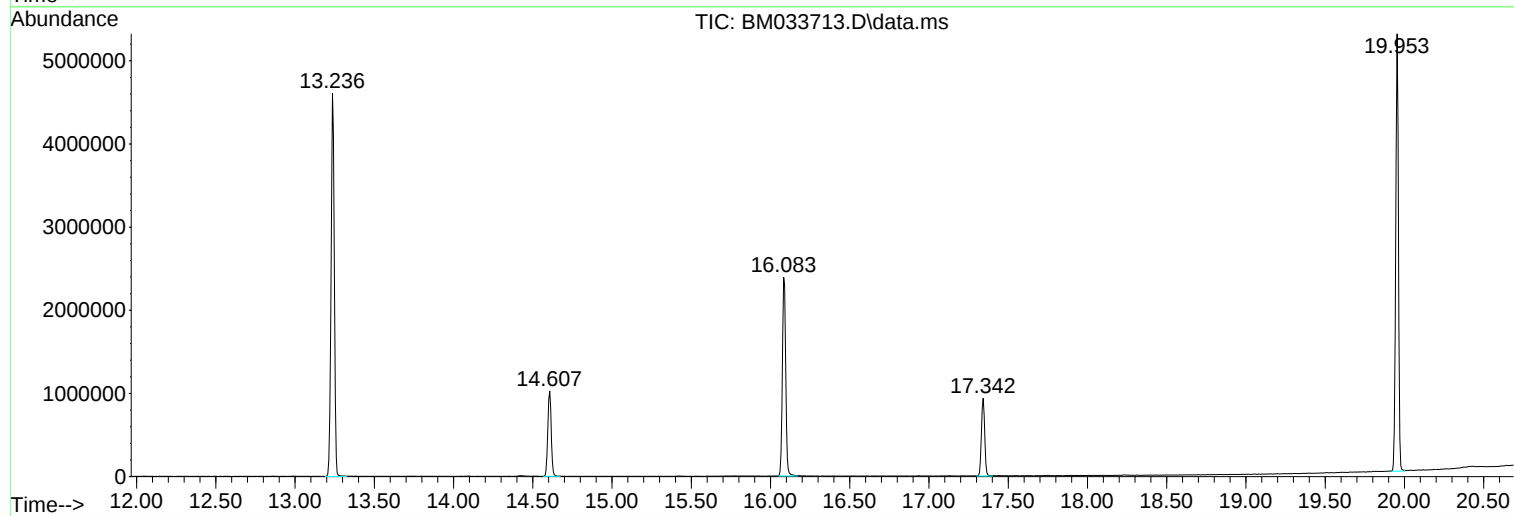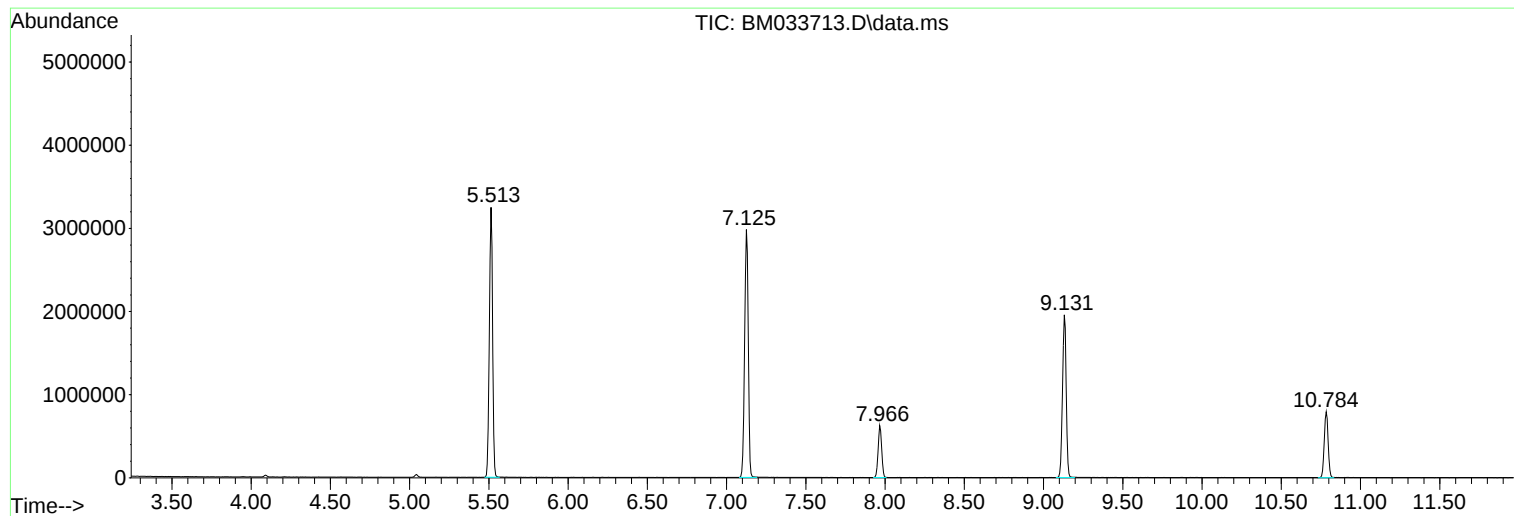

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011322\  
Data File : BM033713.D  
Acq On : 13 Jan 2022 12:01  
Operator : CG/JU  
Sample : PB141980BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB141980BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM010522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011322\  
Data File : BM033713.D  
Acq On : 13 Jan 2022 12:01  
Operator : CG/JU  
Sample : PB141980BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB141980BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM010522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|