
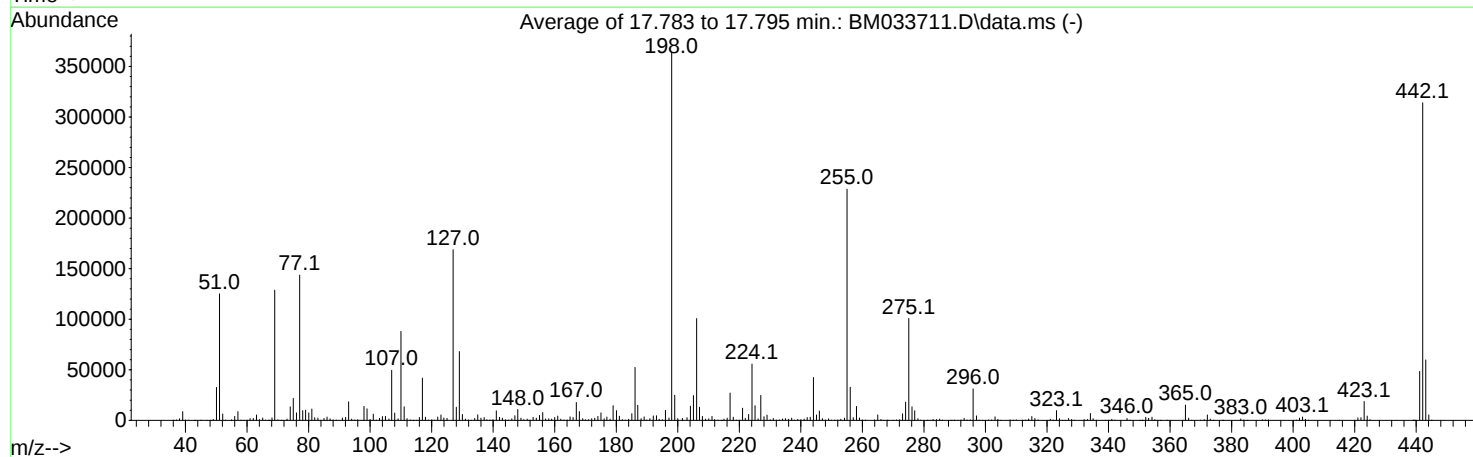


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011322\
 Data File : BM033711.D
 Acq On : 13 Jan 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 13 07:49:01 2022

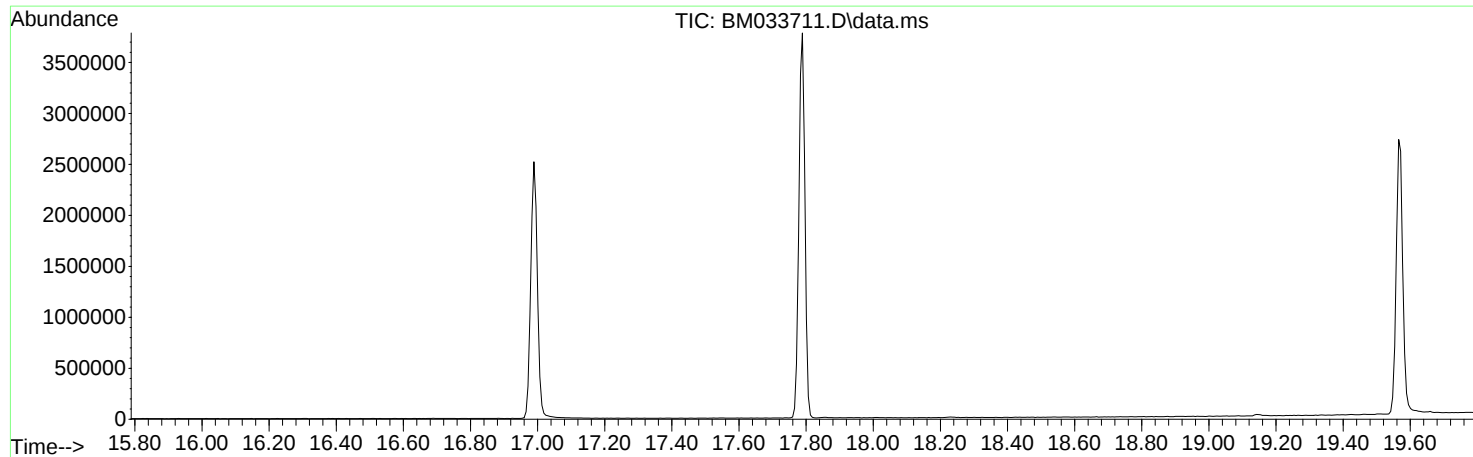




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	125137	PASS
68	69	0.00	2	1.9	2476	PASS
69	198	0.00	100	35.4	128720	PASS
70	69	0.00	2	0.5	624	PASS
127	198	10	80	46.4	168888	PASS
197	198	0.00	2	0.7	2376	PASS
198	198	100	100	100.0	363776	PASS
199	198	5	9	6.8	24832	PASS
275	198	10	60	27.7	100763	PASS
365	198	1	100	4.2	15236	PASS
441	198	0.01	100	13.3	48499	PASS
442	442	50	100	100.0	314112	PASS
443	442	15	24	19.0	59779	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011322\
 Data File : BM033711.D
 Acq On : 13 Jan 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 13 21:28:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 13 07:49:01 2022
 Response via : Initial Calibration

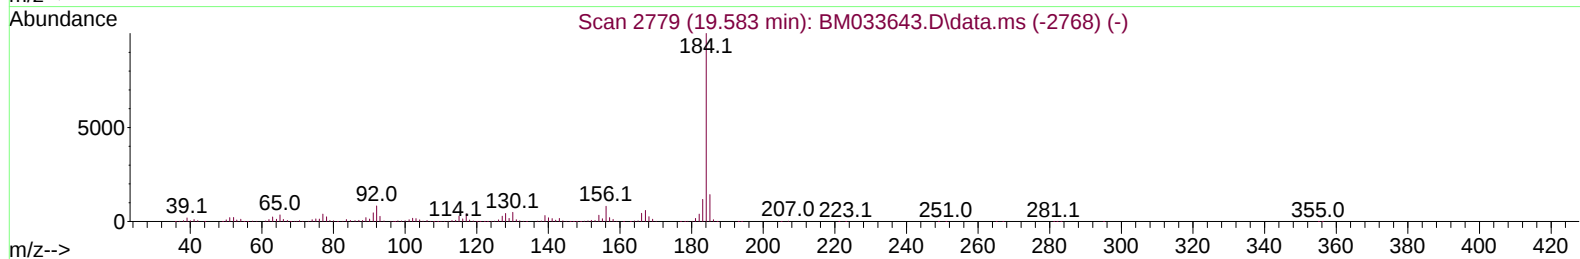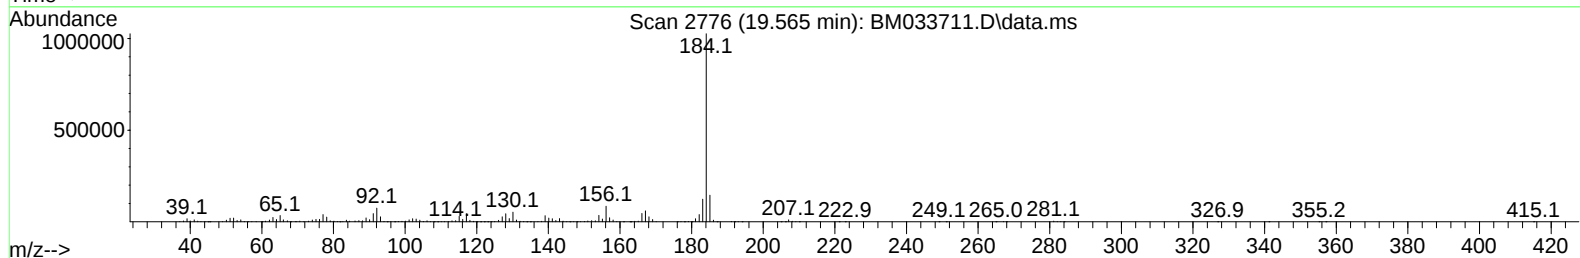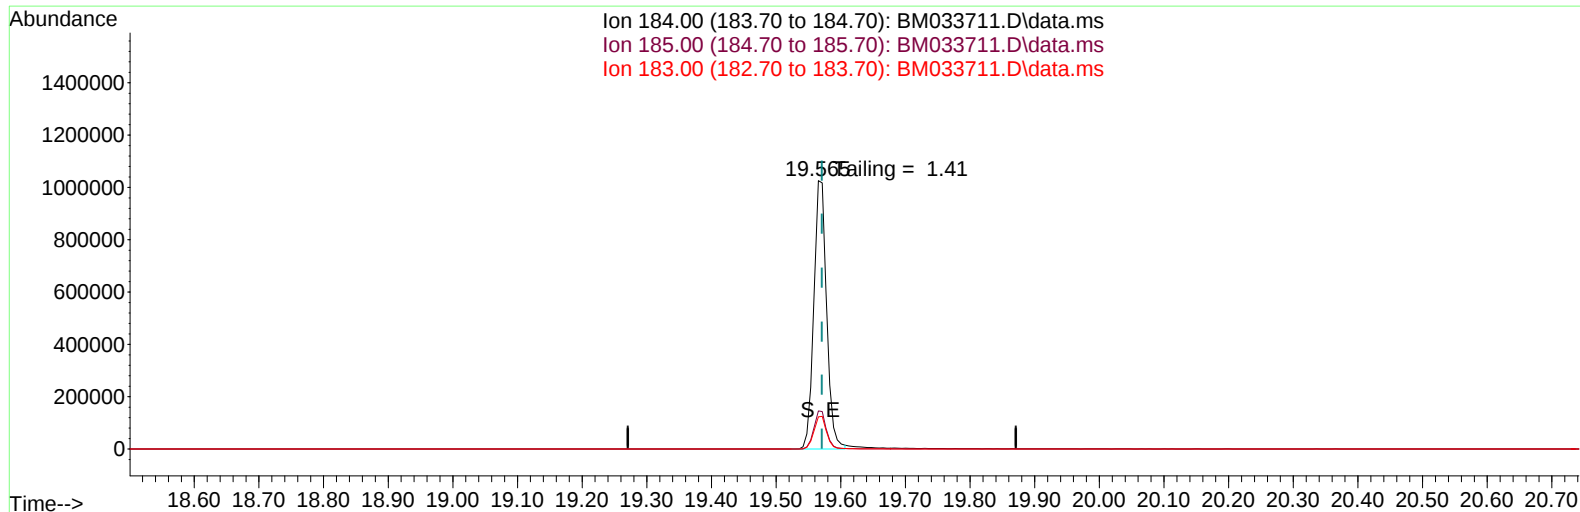

TIC: BM033711.D\data.ms

(77) Benzidine

19.565min (-0.006) 103798.91 ng




response 1445503

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	12.10	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011322\
 Data File : BM033711.D
 Acq On : 13 Jan 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 13 21:28:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 13 07:49:01 2022
 Response via : Initial Calibration

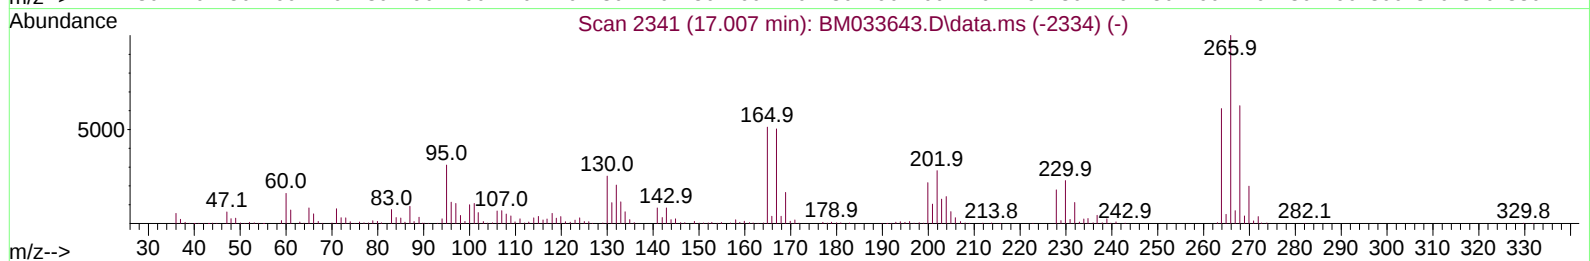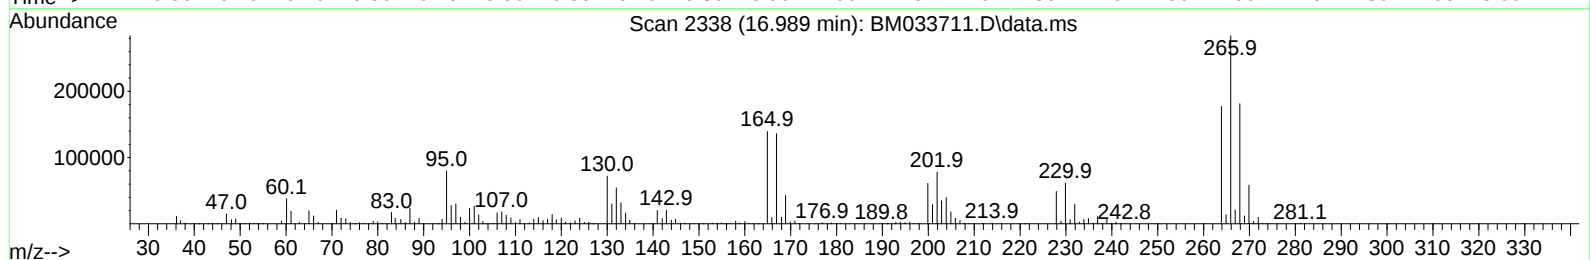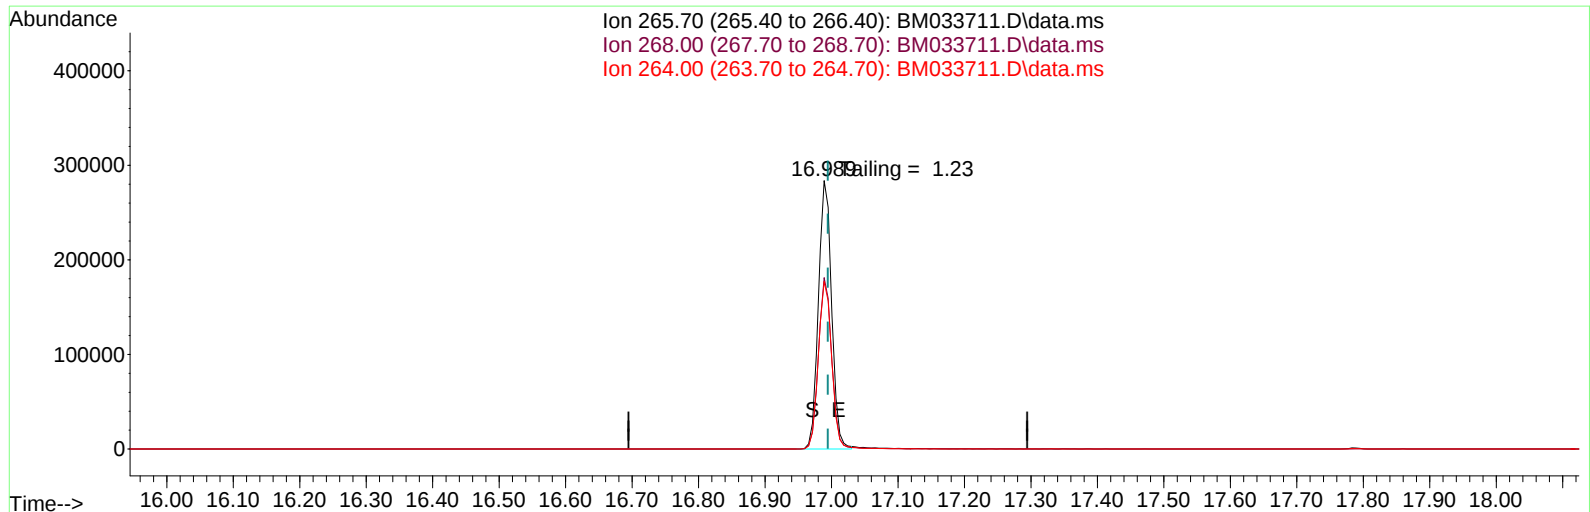

TIC: BM033711.D\data.ms

(70) Pentachlorophenol (C)

16.989min (-0.006) 0.00 ng

response 395622

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.87
264.00	61.40	62.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/13/2022	BNA_M	<u>BM033711.D</u>
Compound Name	Response	Retention Time
DDT	740023	20.806
DDD	88140	20.365
DDE	587	19.859
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
88727	828750	10.71

Instrument :
BNA_M
ClientSampleId :
DFTPP