
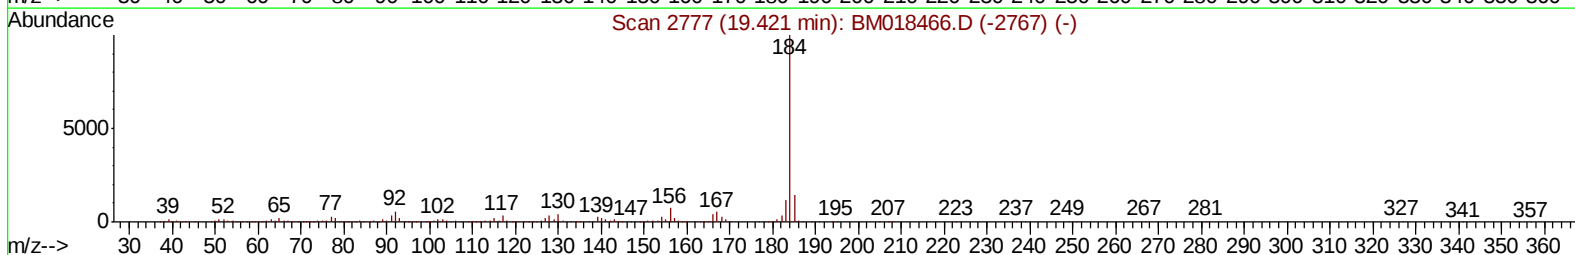
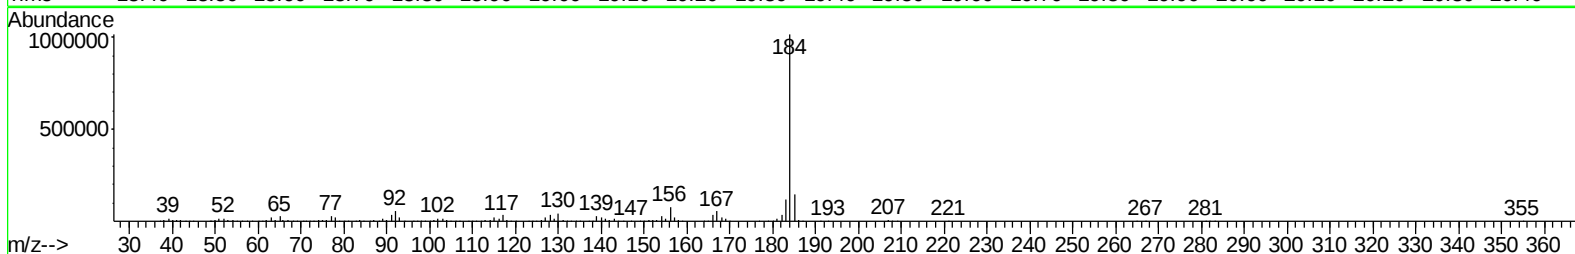


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011419\
 Data File : BM018551.D
 Acq On : 14 Jan 2019 14:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 00:02:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 10 05:57:41 2019
 Response via : Initial Calibration

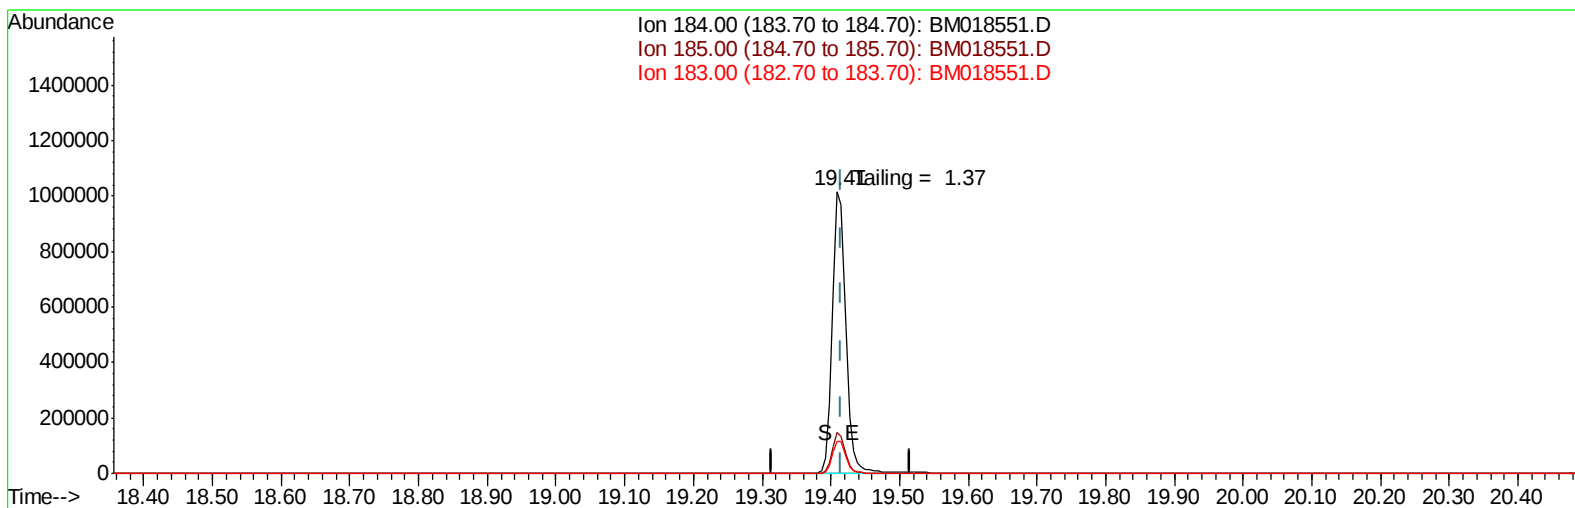

TIC: BM018551.D

(77) Benzidine

19.409min (-0.006) 174361.94ng

response 1373375

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.43
183.00	11.90	11.60
0.00	0.00	0.00

