


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011419\
 Data File : BM018551.D
 Acq On : 14 Jan 2019 14:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

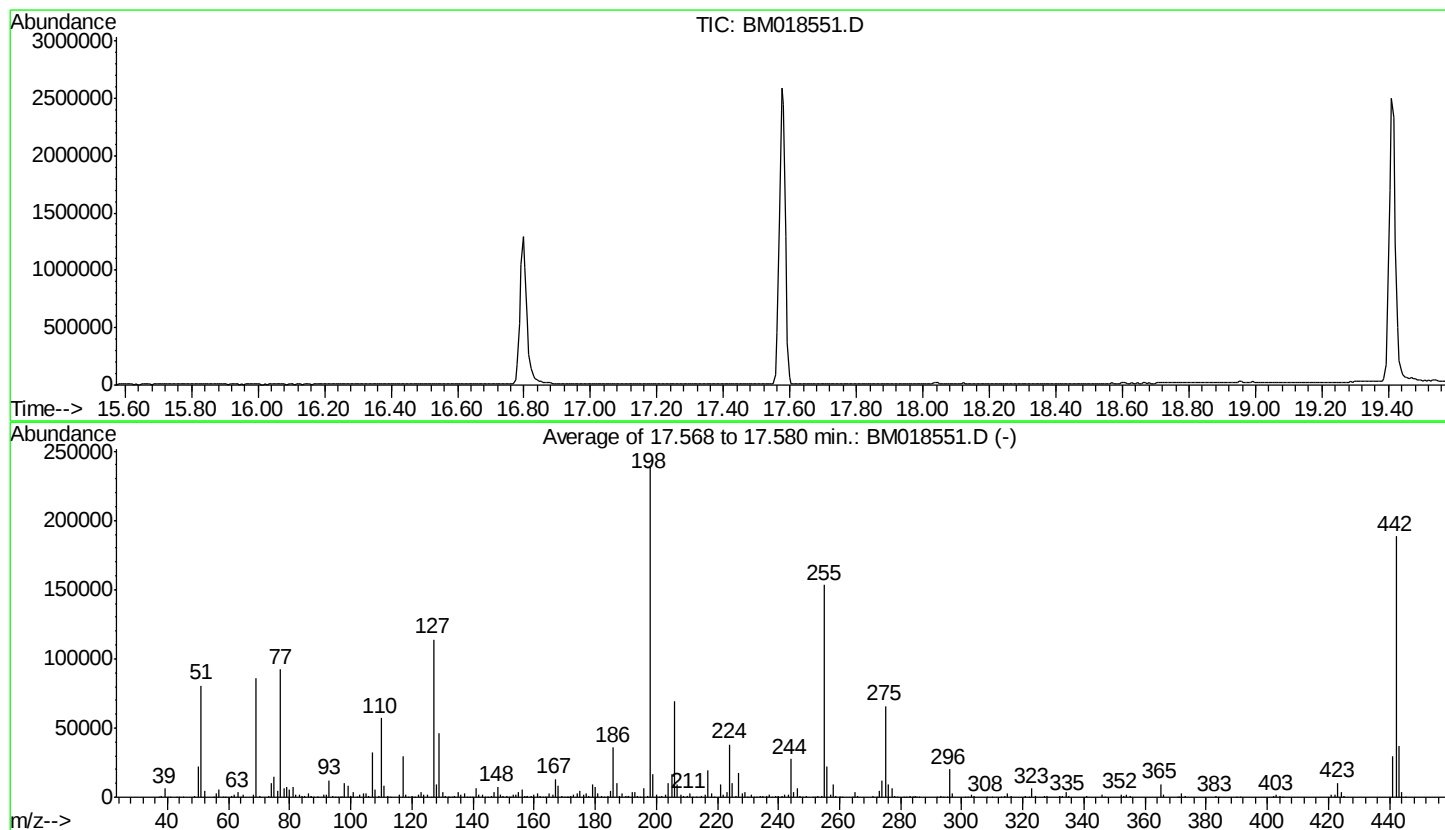

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	80898	PASS
68	69	0.00	2	1.9	1677	PASS
69	198	0.00	100	36.0	86336	PASS
70	69	0.00	2	0.7	579	PASS
127	198	10	80	47.7	114181	PASS
197	198	0.00	2	0.5	1281	PASS
198	198	100	100	100.0	239552	PASS
199	198	5	9	7.0	16672	PASS
275	198	10	60	27.4	65744	PASS
365	198	1	100	4.1	9720	PASS
441	198	0.01	100	12.5	30053	PASS
442	198	50	100	78.7	188464	PASS
443	442	15	24	19.8	37325	PASS