

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011420\
 Data File : BM024470.D
 Acq On : 14 Jan 2020 14:46
 Operator : JU
 Sample : L1067-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFAL5

Quant Time: Jan 14 15:49:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 14 15:42:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	342442	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	1398256	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.12	164	931086	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	2062660	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	2119547	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	2382947	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	41402	5.22	ng/uL	0.00
5) Phenol-d5	6.66	99	149074	5.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	422718	26.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	478814	21.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	291241	13.56	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	320022	30.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	269587	26.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	560960	25.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	44830	1.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.54	166	2360038	35.29	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	2661264	30.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	44778	3.80	ng/ul	0.00
58) Fluorene-d10	15.12	176	1994440	33.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	240614	26.04	ng/ul	0.00
71) Anthracene-d10	16.97	188	3292065	34.08	ng/ul	0.00
79) Pyrene-d10	19.27	212	3901236	34.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	4144397	34.06	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.59	163	120547	1.757	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011420\
Data File : BM024470.D
Acq On : 14 Jan 2020 14:46
Operator : JU
Sample : L1067-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFAL5

Quant Time: Jan 14 15:49:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 14 15:42:37 2020
Response via : Initial Calibration

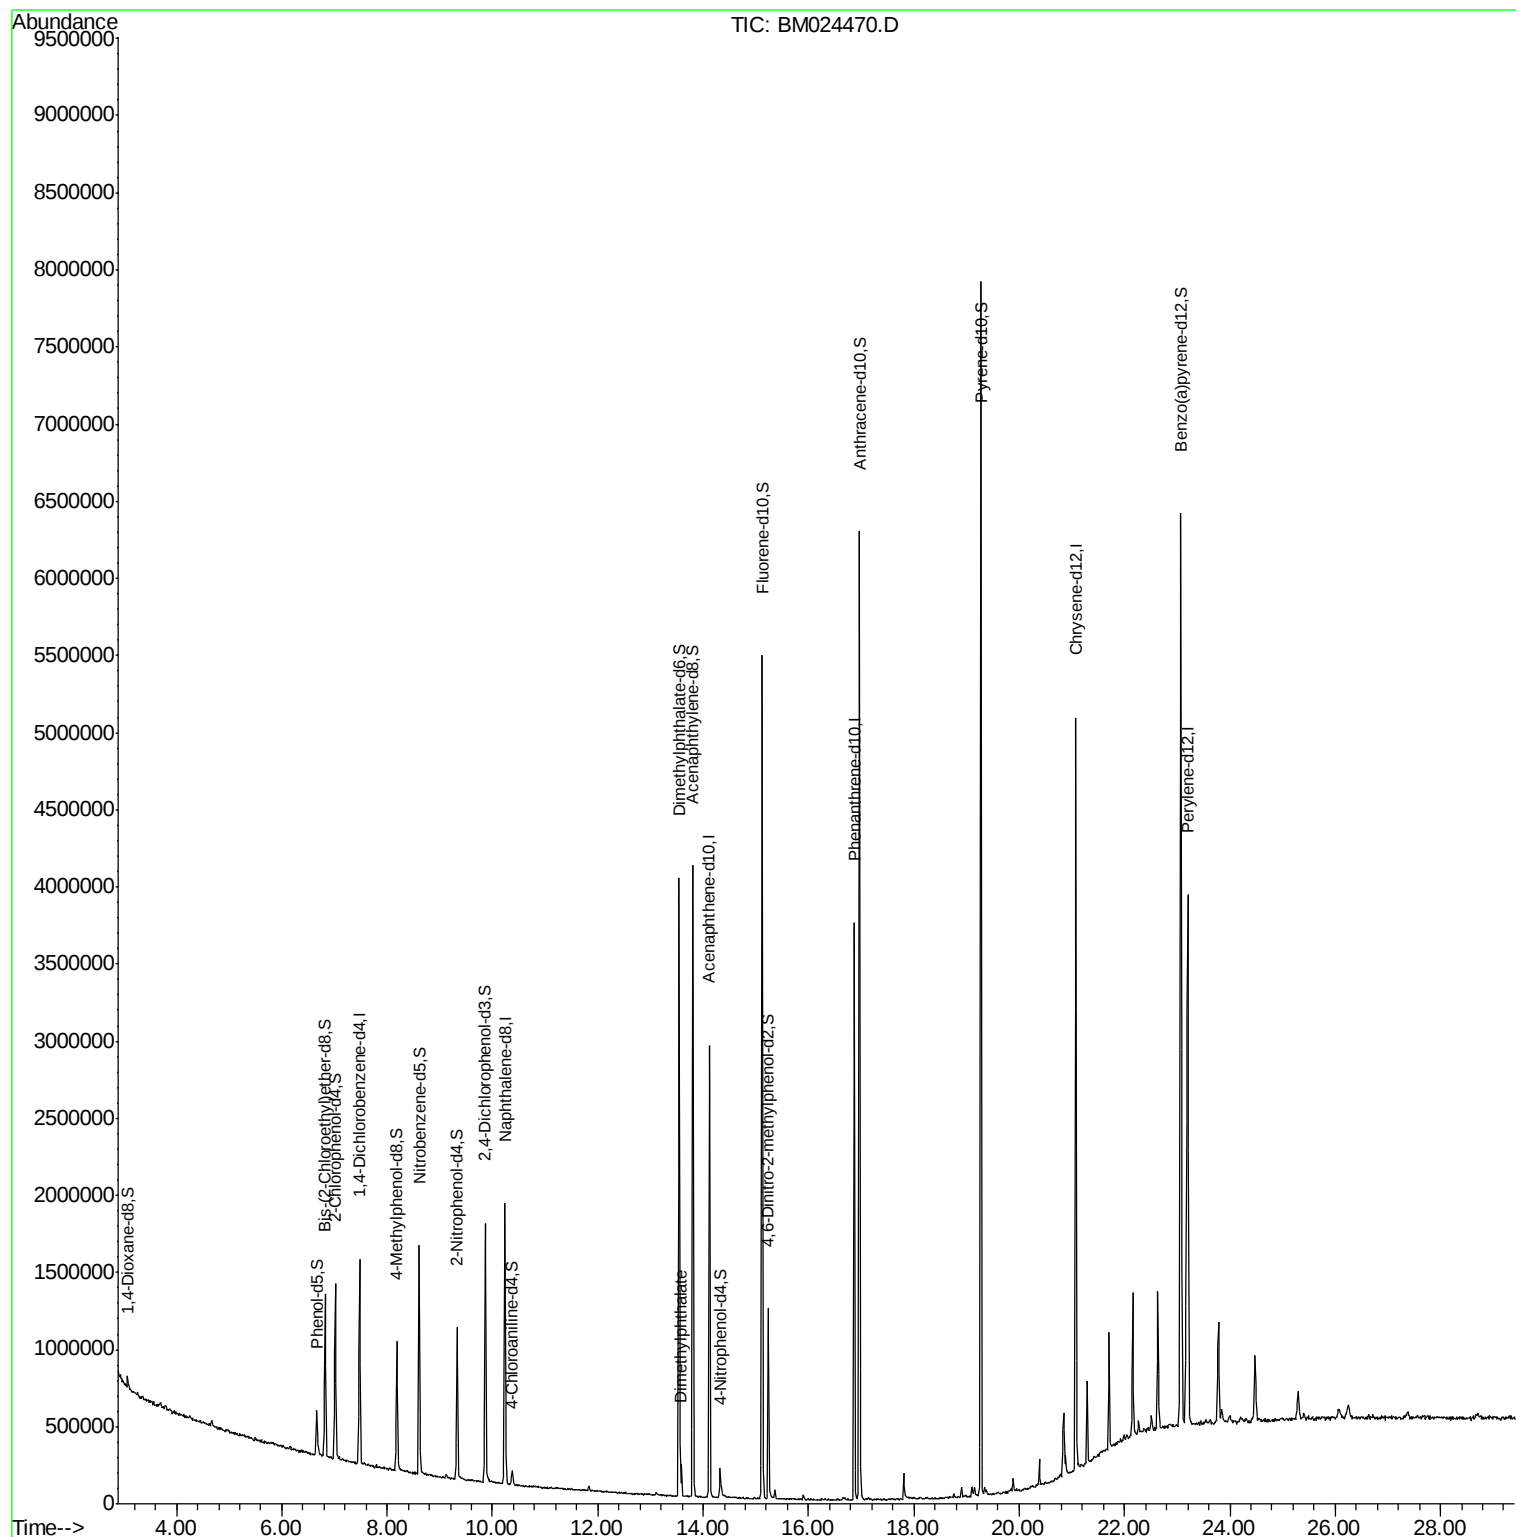

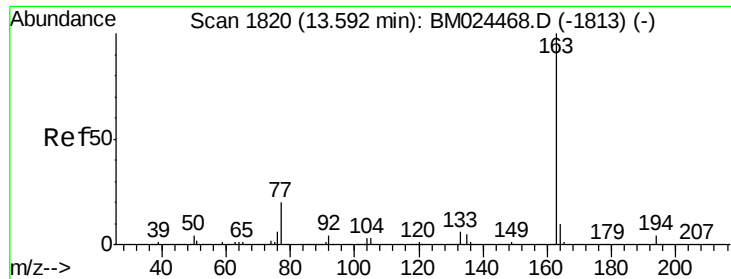

#45

Dimethylphthalate

Concen: 1.757 ng/ul

RT: 13.59 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BM024470.D

Acq: 14 Jan 2020 14:46

Instrument :

BNA_M

ClientSampleId :

BFAL5


Tot Ion:163 Resp: 120547

Ion Ratio Lower Upper

163 100

194 3.2 3.2 4.8

164 10.5 8.2 12.4

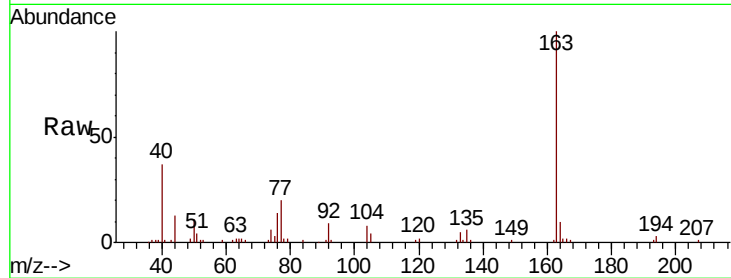

Abundance Ion 163.00 (162.70 to 163.70): E

120000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

