

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011420\
 Data File : BM024472.D
 Acq On : 14 Jan 2020 15:58
 Operator : JU
 Sample : L1067-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFAL9

Quant Time: Jan 14 16:41:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 14 15:42:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	386209	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	1589338	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.12	164	1041331	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	2261986	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1991722	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	1943681	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	51554	5.76	ng/uL	0.00
5) Phenol-d5	6.66	99	185536	6.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	517900	29.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	589613	23.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	376514	15.54	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	396819	33.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	332021	29.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	728558	29.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	48563	1.72	ng/ul	0.00
44) Dimethylphthalate-d6	13.55	166	2855407	38.17	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	3287235	34.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	55609	4.22	ng/ul	0.00
58) Fluorene-d10	15.12	176	2425293	36.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	282491	27.87	ng/ul	0.00
71) Anthracene-d10	16.97	188	3842826	36.27	ng/ul	0.00
79) Pyrene-d10	19.27	212	4313936	40.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	3599493	36.27	ng/ul	0.00

Target Compounds


				Ovalue	
45) Dimethylphthalate	13.59	163	162238	2.114	ng/ul# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011420\
Data File : BM024472.D
Acq On : 14 Jan 2020 15:58
Operator : JU
Sample : L1067-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFAL9

Quant Time: Jan 14 16:41:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 14 15:42:37 2020
Response via : Initial Calibration

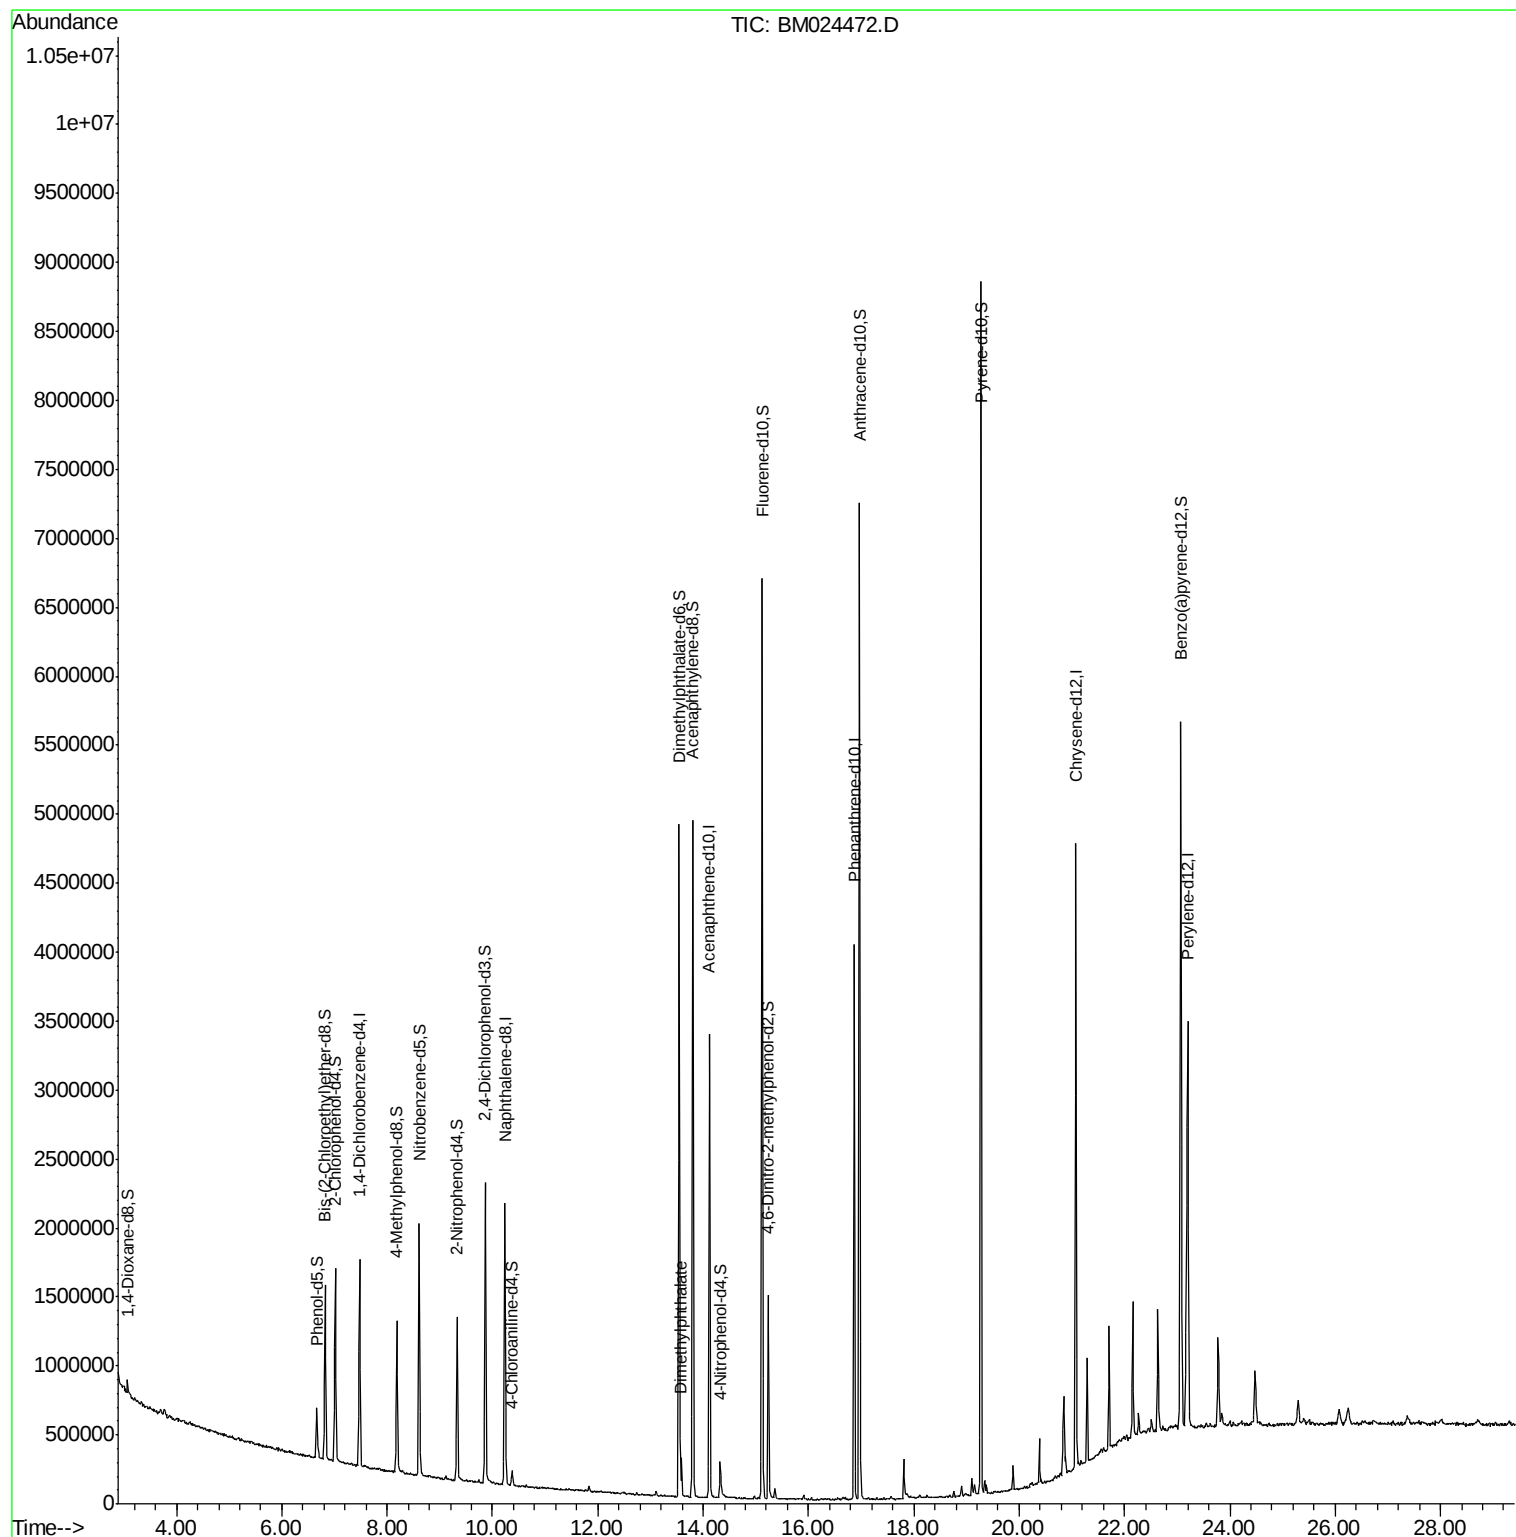

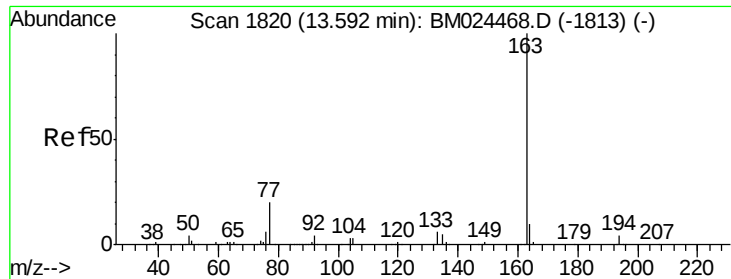

#45

Dimethylphthalate

Concen: 2.114 ng/ul

RT: 13.59 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BM024472.D

Acq: 14 Jan 2020 15:58

Instrument :

BNA_M

ClientSampleId :

BFAL9


Tot Ion:163 Resp: 162238

Ion Ratio Lower Upper

163 100

194 5.4 3.2 4.8#

164 11.1 8.2 12.4

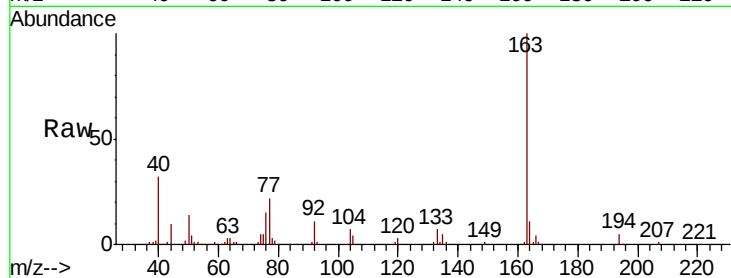

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

