
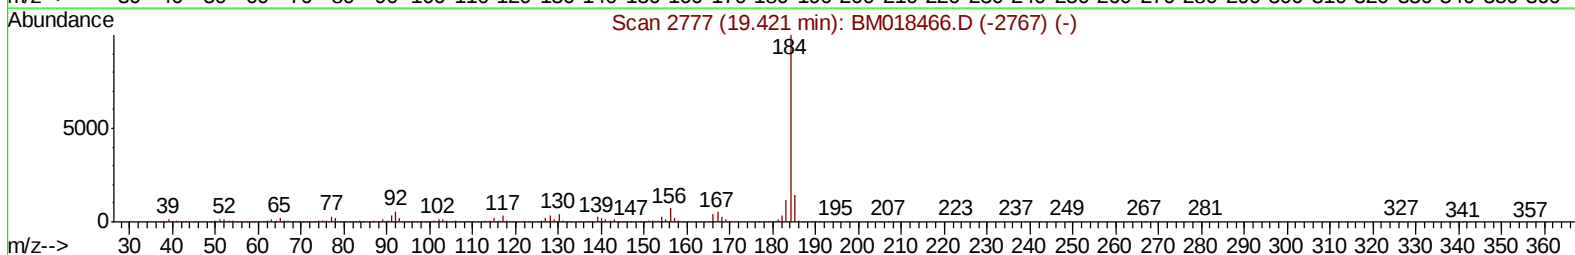
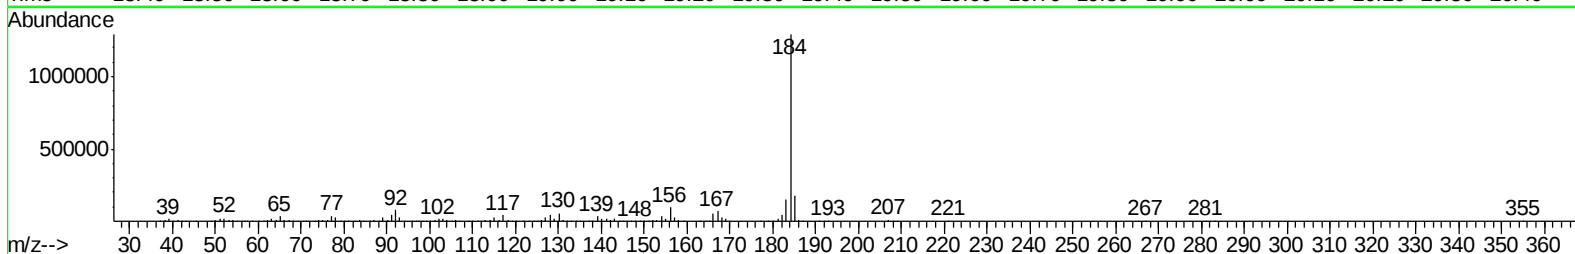


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM011519\
 Data File : BM018563.D
 Acq On : 15 Jan 2019 15:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:27:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 10 05:57:41 2019
 Response via : Initial Calibration

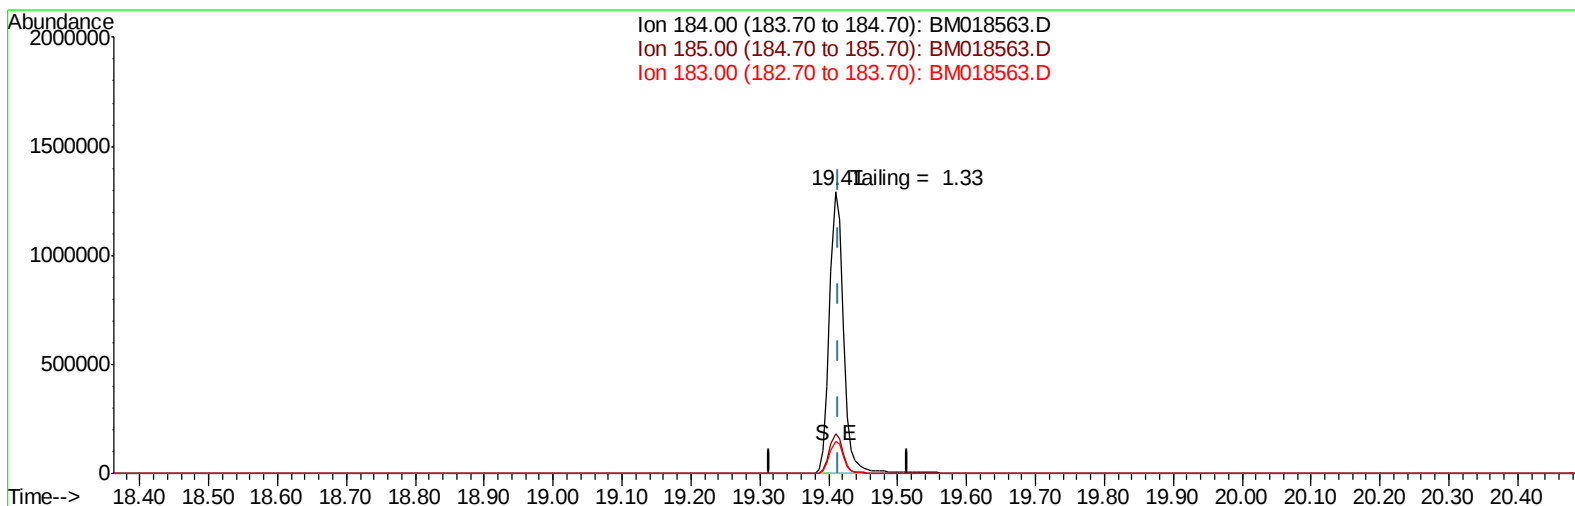

TIC: BM018563.D

(77) Benzidine




19.409min (-0.006) 151803.27ng

response 1810402

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.99
183.00	11.90	11.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM011519\
Data File : BM018563.D
Acq On : 15 Jan 2019 15:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:27:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

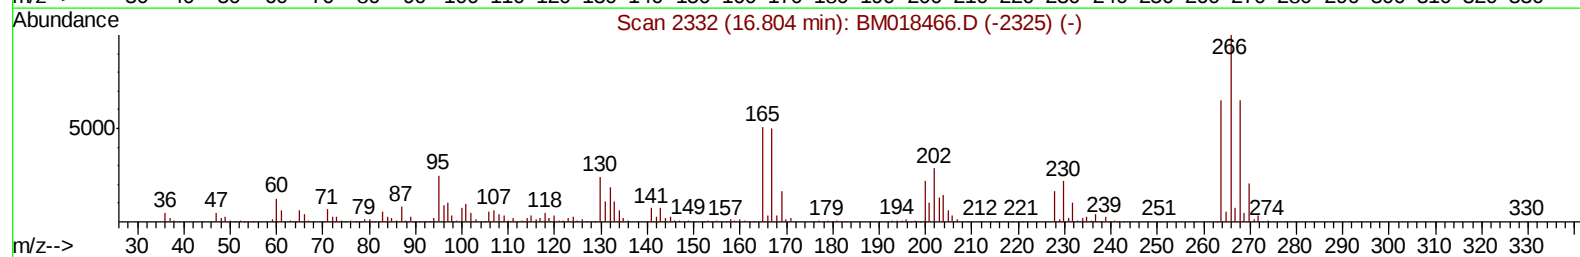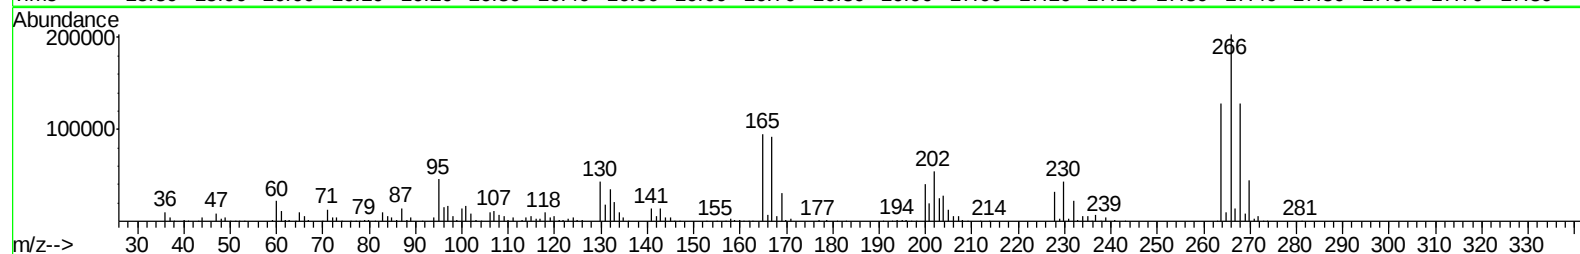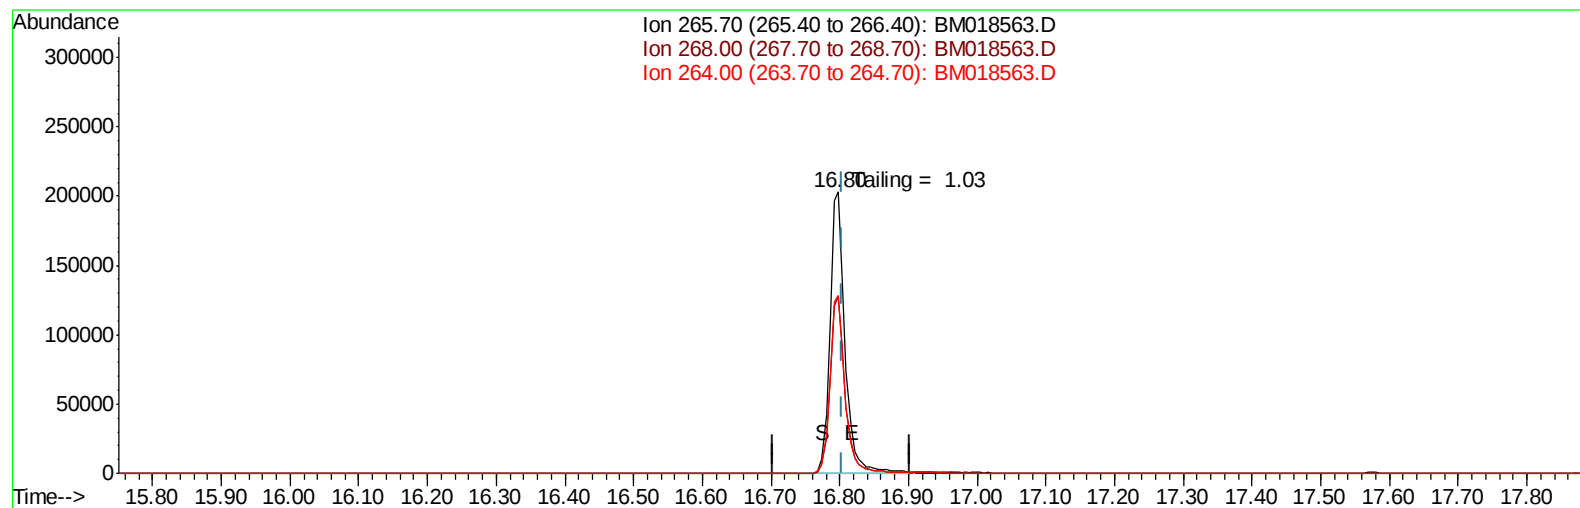

TIC: BM018563.D

(70) Pentachlorophenol (C)

16.798min (-0.006) 0.00ng

response 310133

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.92
264.00	62.60	63.00
0.00	0.00	0.00