


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011519\
 Data File : BM018563.D
 Acq On : 15 Jan 2019 15:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

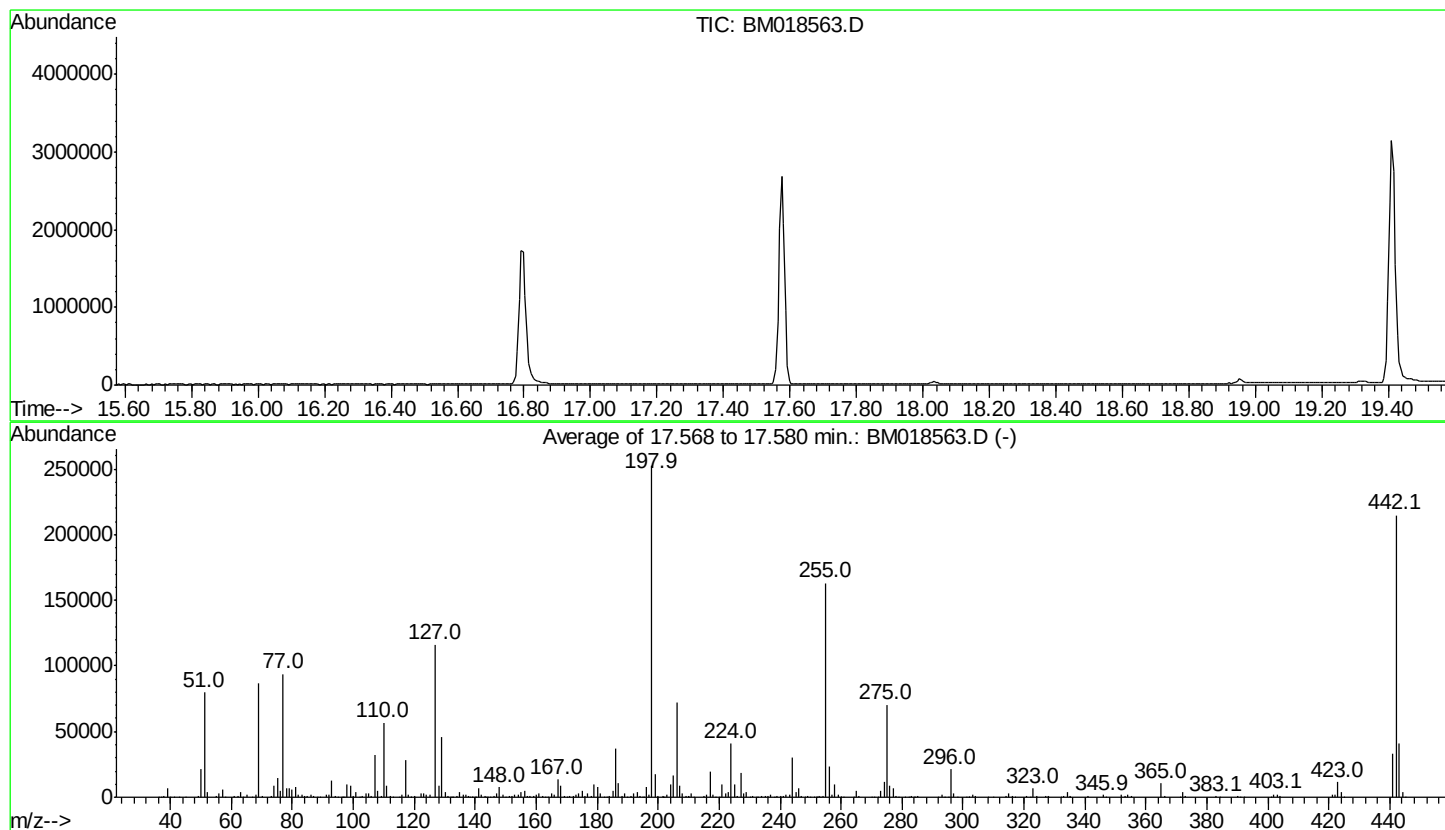

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	79904	PASS
68	69	0.00	2	2.0	1729	PASS
69	198	0.00	100	34.4	86960	PASS
70	69	0.00	2	0.7	577	PASS
127	198	10	80	46.1	116349	PASS
197	198	0.00	2	0.6	1593	PASS
198	198	100	100	100.0	252586	PASS
199	198	5	9	6.9	17316	PASS
275	198	10	60	28.0	70661	PASS
365	198	1	100	4.1	10277	PASS
441	198	0.01	100	13.0	32861	PASS
442	198	50	100	84.9	214570	PASS
443	442	15	24	19.0	40834	PASS