

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM011619\  
 Data File : BM018587.D  
 Acq On : 16 Jan 2019 17:26  
 Operator : JU/SJ  
 Sample : K1149-01  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SW001-190114-01

Quant Time: Jan 17 01:09:01 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM010919.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jan 10 05:57:41 2019  
 Response via : Initial Calibration


| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.75  | 152  | 111876   | 20.00  | ng    | -0.02    |
| 21) Naphthalene-d8          | 10.54 | 136  | 464227   | 20.00  | ng    | -0.01    |
| 39) Acenaphthene-d10        | 14.39 | 164  | 275696   | 20.00  | ng    | -0.02    |
| 64) Phenanthrene-d10        | 17.14 | 188  | 672337   | 20.00  | ng    | -0.01    |
| 76) Chrysene-d12            | 21.34 | 240  | 1004758  | 20.00  | ng    | -0.01    |
| 87) Perylene-d12            | 23.62 | 264  | 1266354  | 20.00  | ng    | -0.02    |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.33  | 112  | 411057   | 67.84  | ng    | -0.02    |
| 7) Phenol-d6                | 6.92  | 99   | 339713   | 44.14  | ng    | -0.01    |
| 23) Nitrobenzene-d5         | 8.91  | 82   | 653726   | 81.63  | ng    | -0.01    |
| 42) 2,4,6-Tribromophenol    | 15.89 | 330  | 531329   | 151.36 | ng    | -0.01    |
| 45) 2-Fluorobiphenyl        | 13.01 | 172  | 1708590  | 80.87  | ng    | -0.01    |
| 79) Terphenyl-d14           | 19.77 | 244  | 3413752  | 71.62  | ng    | -0.01    |
| Target Compounds            |       |      |          |        |       | Qvalue   |
| 10) Phenol                  | 6.95  | 94   | 51757    | 6.619  | ng    | 96       |
| 17) 2-Methylphenol          | 8.19  | 107  | 21934    | 4.132  | ng    | 96       |
| 20) 3+4-Methylphenols       | 8.52  | 107  | 43197    | 5.895  | ng    | 88       |
| 31) Naphthalene             | 10.59 | 128  | 340798   | 15.243 | ng    | 99       |
| 32) Benzoic acid            | 9.86  | 122  | 122      | 6.530  | ng    | # 28     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM011619\  
Data File : BM018587.D  
Acq On : 16 Jan 2019 17:26  
Operator : JU/SJ  
Sample : K1149-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SW001-190114-01

Quant Time: Jan 17 01:09:01 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM010919.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jan 10 05:57:41 2019  
Response via : Initial Calibration

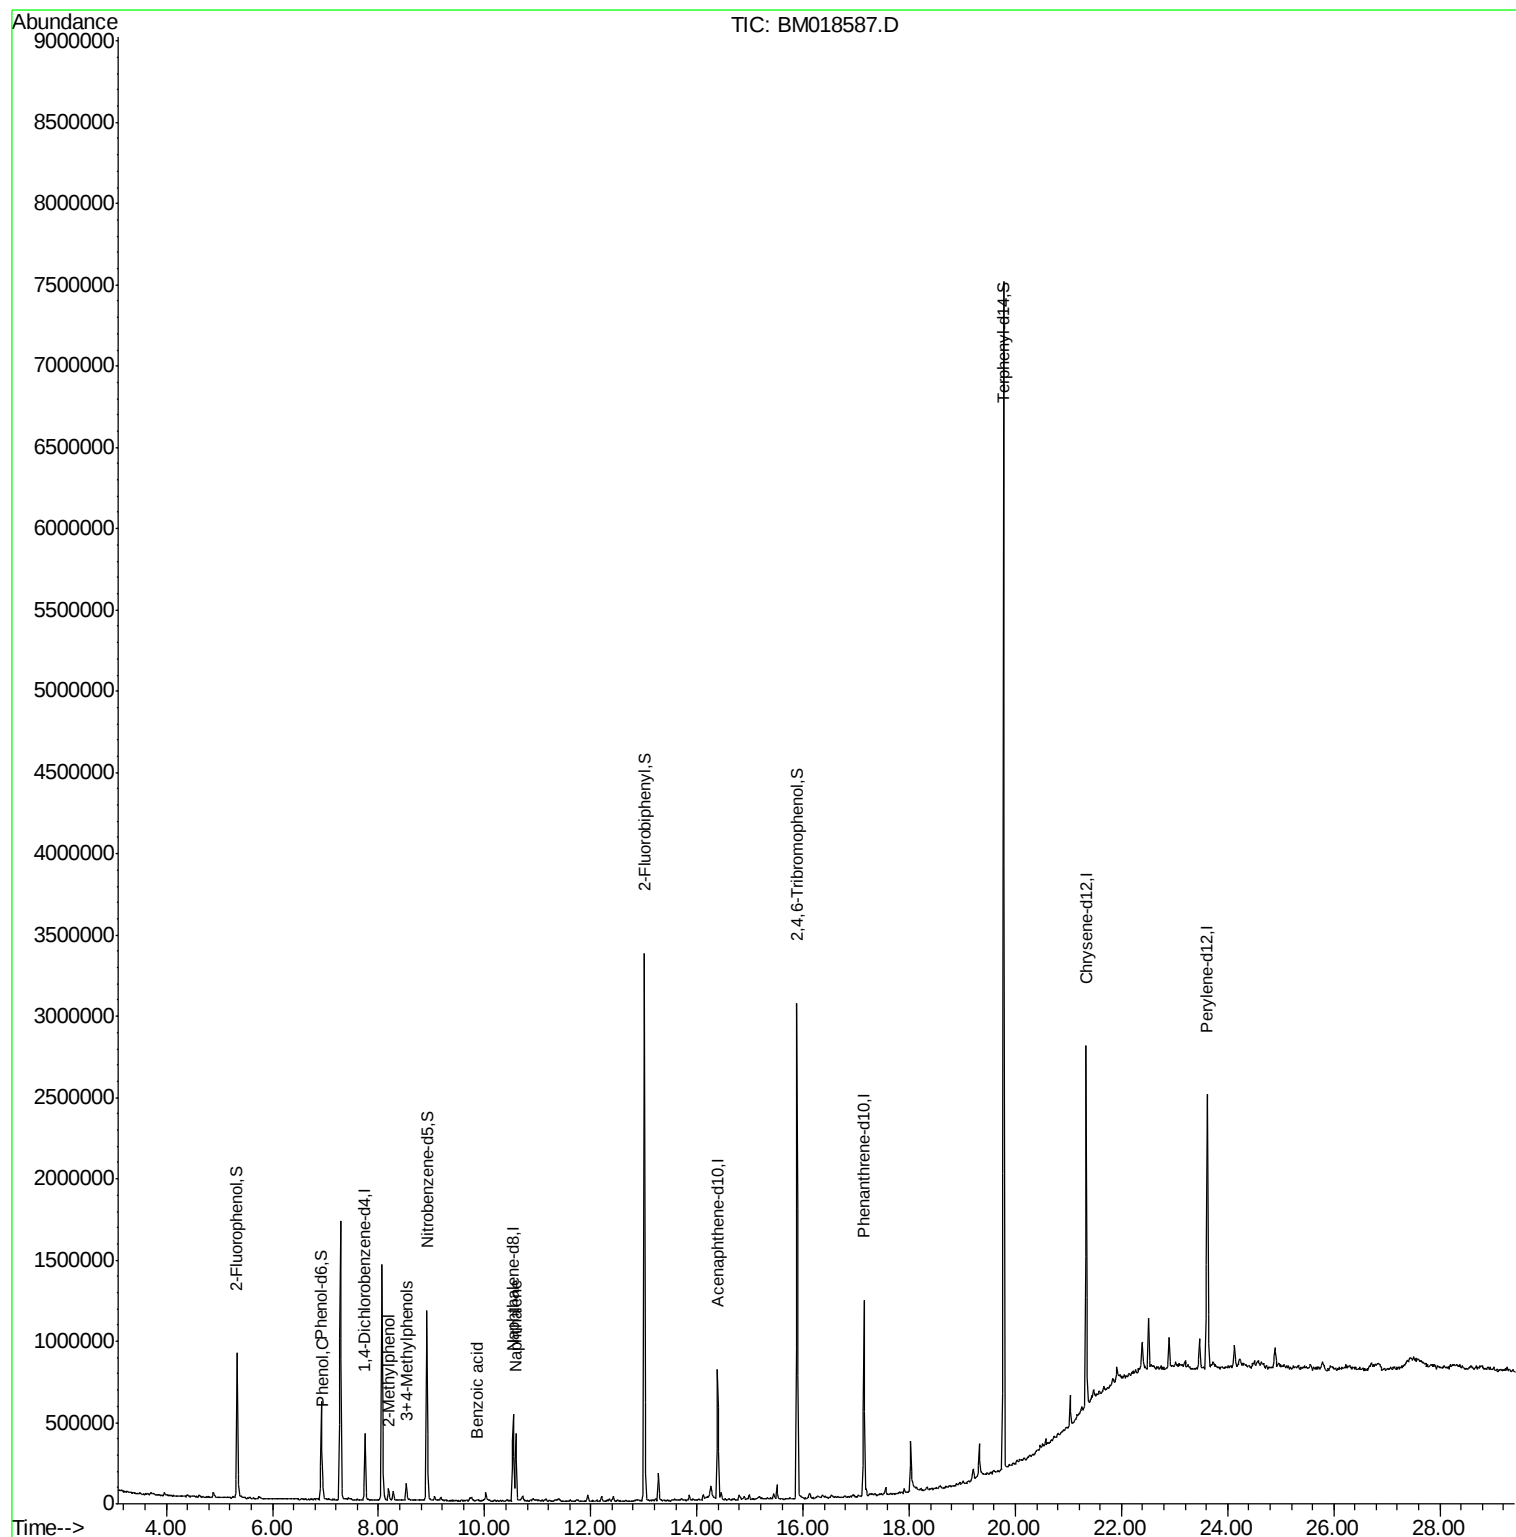


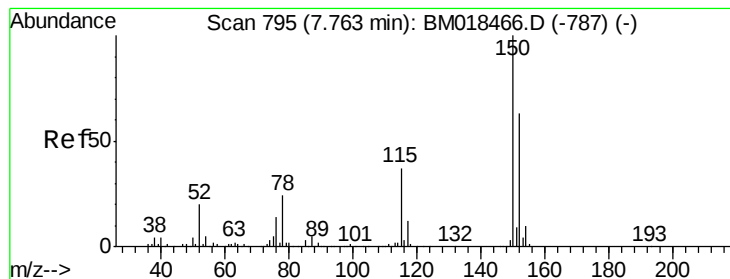




#1  
 1,4-Dichlorobenzene-d4  
 Concen: 20.000 ng  
 RT: 7.75 min Scan# 792  
 Delta R.T. -0.02 min  
 Lab File: BM018587.D  
 Acq: 16 Jan 2019 17:26

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SW001-190114-01

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 152     | 100   |       |       |
| 150     | 153.5 | 126.9 | 190.3 |
| 115     | 58.8  | 45.5  | 68.3  |




Abundance Ion 152.00 (151.70 to 152.70): E  
 Ion 150.00 (149.70 to 150.70): E  
 Ion 115.00 (114.70 to 115.70): E

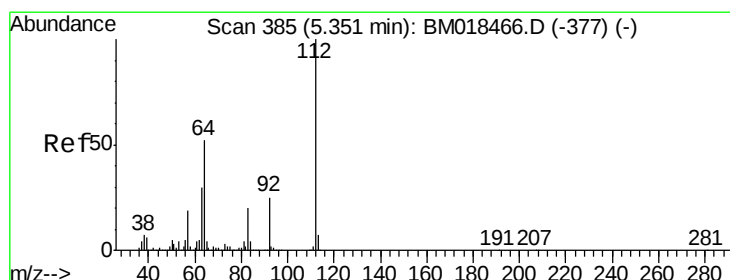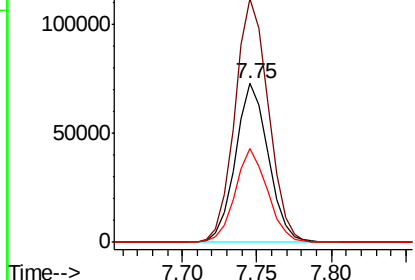
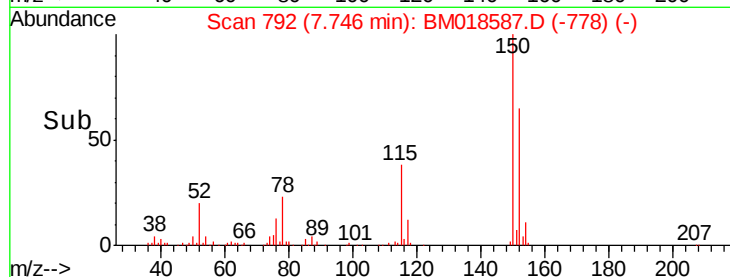



#5  
 2-Fluorophenol  
 Concen: 67.844 ng  
 RT: 5.33 min Scan# 382  
 Delta R.T. -0.02 min  
 Lab File: BM018587.D  
 Acq: 16 Jan 2019 17:26

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 112     | 100   |       |       |
| 64      | 55.0  | 46.5  | 69.7  |
| 63      | 29.8  | 25.2  | 37.8  |



Abundance Ion 112.00 (111.70 to 112.70): E  
 Ion 64.00 (63.70 to 64.70): BM0  
 Ion 63.00 (62.70 to 63.70): BM0

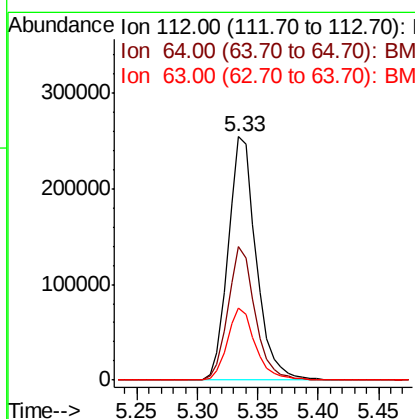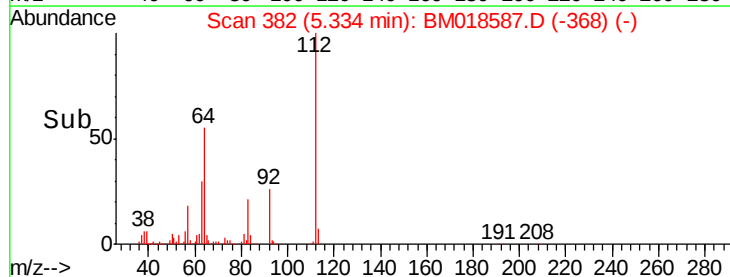

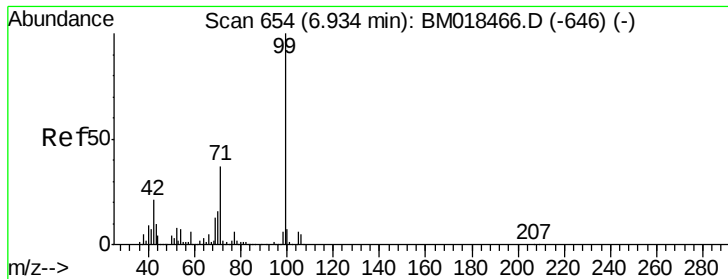

#7

Phenol-d6

Concen: 44.145 ng

RT: 6.92 min Scan# 652

Delta R.T. -0.01 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26

Instrument :

BNA\_M

ClientSampleId :

SW001-190114-01


Tgt Ion: 99 Resp: 339713

Ion Ratio Lower Upper

99 100

42 19.3 17.3 25.9

71 35.9 28.0 42.0



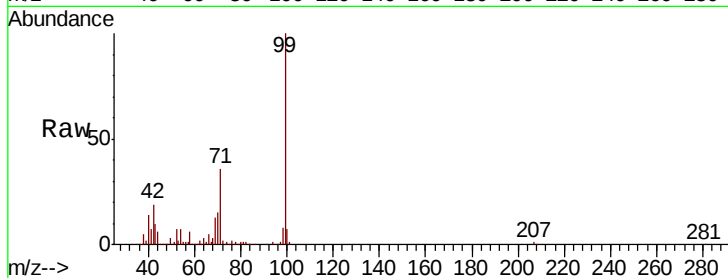


Abundance Ion 99.00 (98.70 to 99.70): BM018466.D (-646) (-)

Ion 42.00 (41.70 to 42.70): BM018466.D (-646) (-)

Ion 71.00 (70.70 to 71.70): BM018466.D (-646) (-)

Time-->

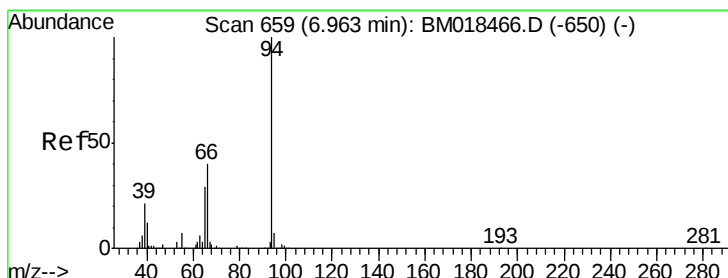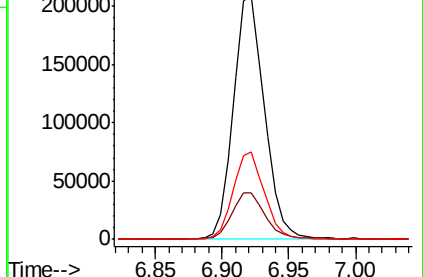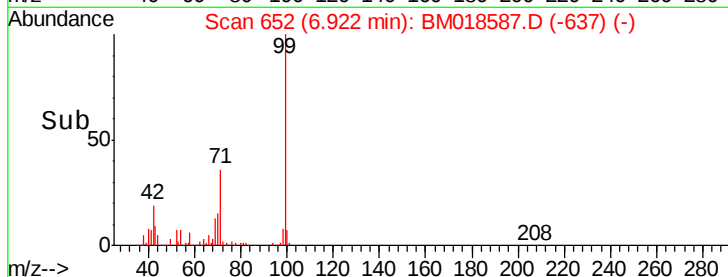

#10

Phenol

Concen: 6.619 ng

RT: 6.95 min Scan# 656

Delta R.T. -0.02 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26


Tgt Ion: 94 Resp: 51757

Ion Ratio Lower Upper

94 100

65 29.6 9.4 49.4

66 43.5 19.1 59.1


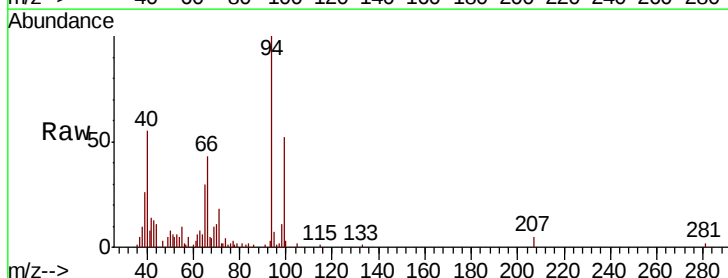



Abundance Ion 94.00 (93.70 to 94.70): BM018466.D (-650) (-)

Ion 65.00 (64.70 to 65.70): BM018466.D (-650) (-)

Ion 66.00 (65.70 to 66.70): BM018466.D (-650) (-)

Time-->

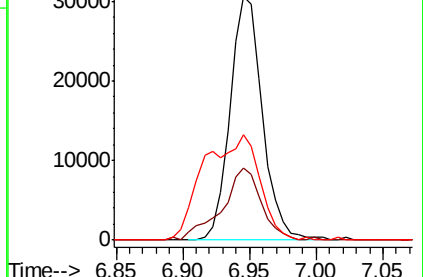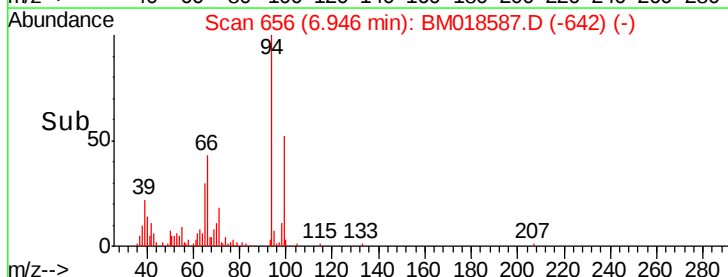

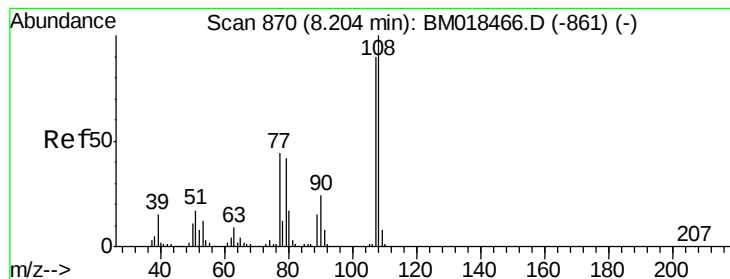

#17

2-Methylphenol

Concen: 4.132 ng

RT: 8.19 min Scan# 868

Delta R.T. -0.02 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26

Instrument :

BNA\_M

ClientSampleId :

SW001-190114-01

Tgt Ion:107 Resp: 21934


Ion Ratio Lower Upper

107 100

108 113.8 87.5 131.3

77 48.7 37.3 55.9

79 49.9 36.4 54.6






Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 79.00 (78.70 to 79.70): BM0

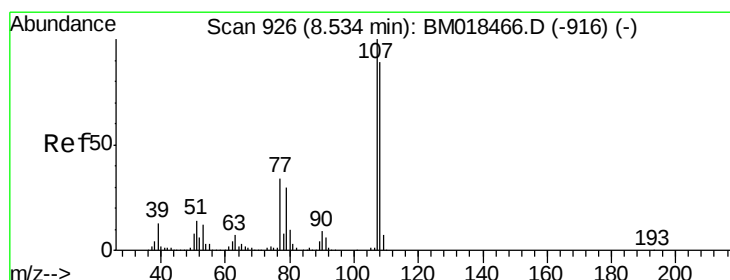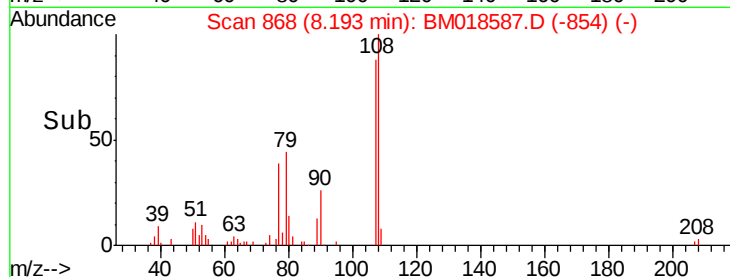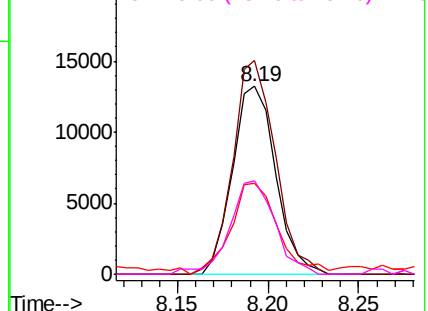

#20

3+4-Methylphenols

Concen: 5.895 ng

RT: 8.52 min Scan# 924

Delta R.T. -0.01 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26

Tgt Ion:107 Resp: 43197


Ion Ratio Lower Upper

107 100

108 98.5 66.8 106.8

77 35.9 13.3 53.3

79 38.2 8.8 48.8






Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 79.00 (78.70 to 79.70): BM0

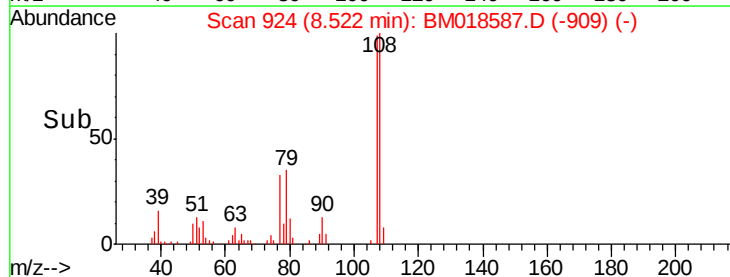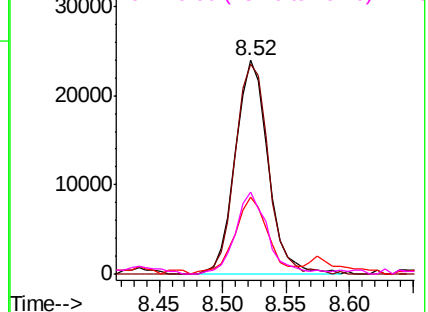

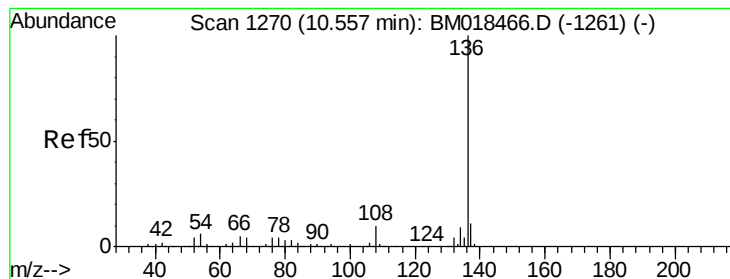

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.54 min Scan# 1267

Delta R.T. -0.01 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26

Instrument :

BNA\_M

ClientSampleId :

SW001-190114-01

Tgt Ion: 136 Resp: 464227





Ion Ratio Lower Upper

136 100

137 11.2 8.5 12.7

54 6.0 6.0 9.0

68 4.1 4.5 6.7#

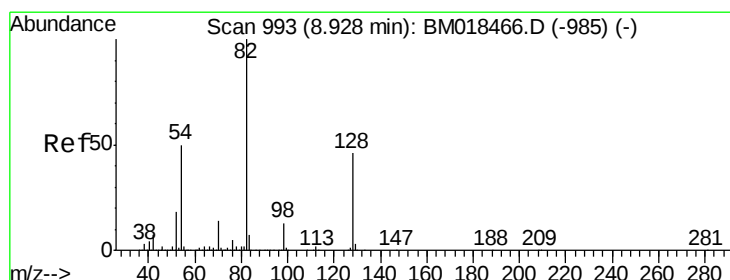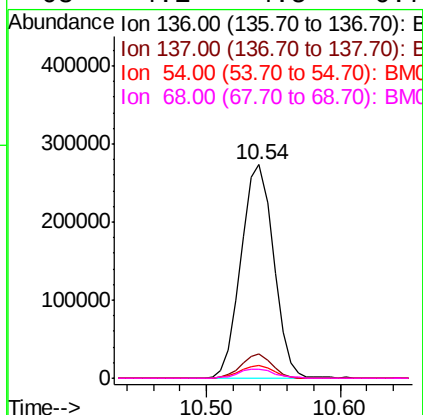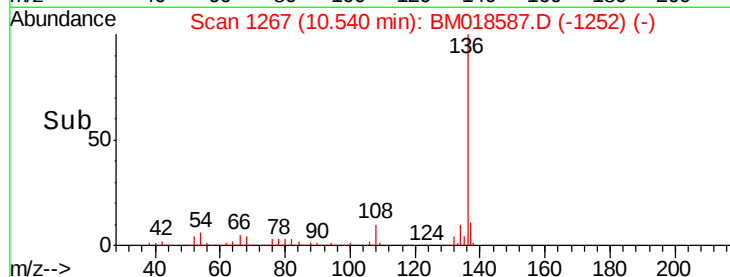

#23

Nitrobenzene-d5

Concen: 81.635 ng

RT: 8.91 min Scan# 990

Delta R.T. -0.01 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26




Tgt Ion: 82 Resp: 653726


Ion Ratio Lower Upper

82 100

128 47.2 36.3 54.5

54 49.1 41.7 62.5


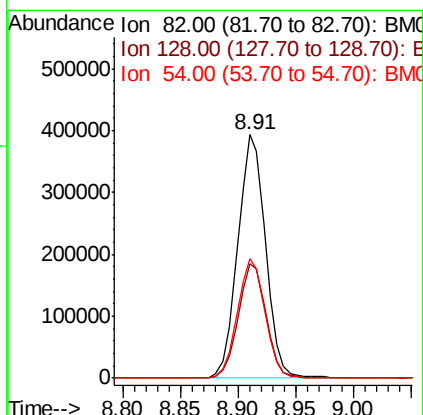
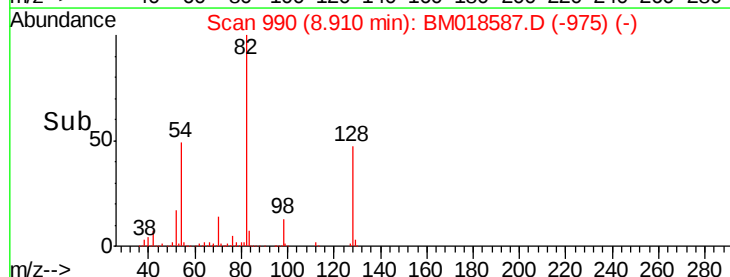



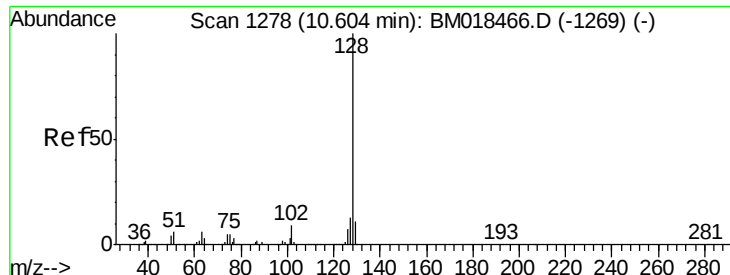

#31  
Naphthalene  
Concen: 15.243 ng  
RT: 10.59 min Scan# 1275  
Delta R.T. -0.02 min  
Lab File: BM018587.D  
Acq: 16 Jan 2019 17:26




Instrument :  
BNA\_M  
ClientSampleId :  
SW001-190114-01


Tgt Ion:128 Resp: 340798  
Ion Ratio Lower Upper  
128 100  
129 11.3 8.7 13.1  
127 12.8 10.8 16.2

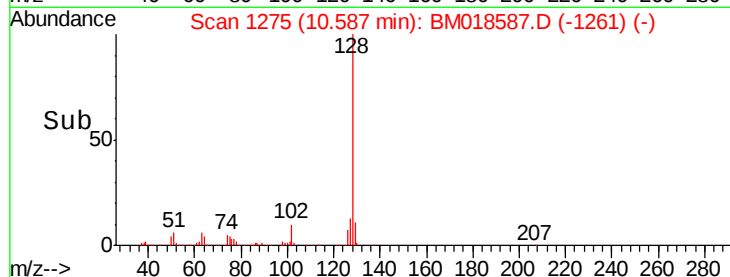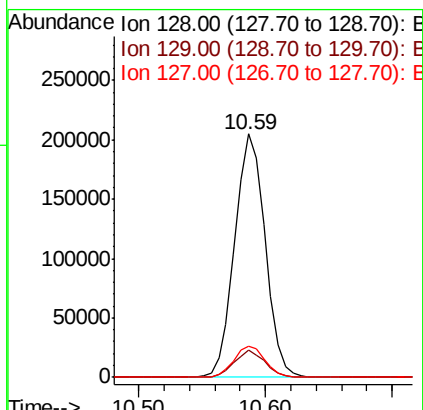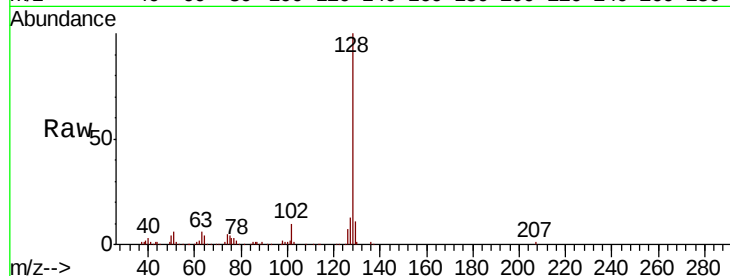

#32  
Benzoic acid  
Concen: 6.530 ng  
RT: 9.86 min Scan# 1152  
Delta R.T. -0.04 min  
Lab File: BM018587.D  
Acq: 16 Jan 2019 17:26

Tgt Ion:122 Resp: 122  
Ion Ratio Lower Upper  
122 100  
105 0.0 100.4 140.4#  
77 115.0 71.7 111.7#

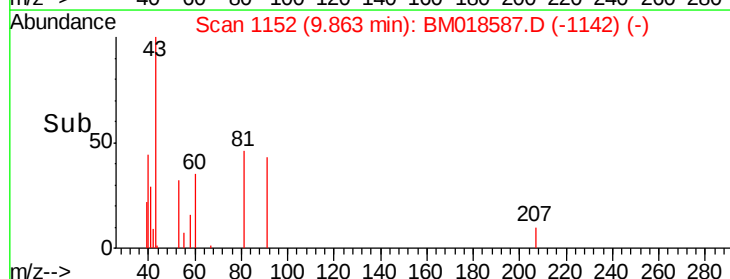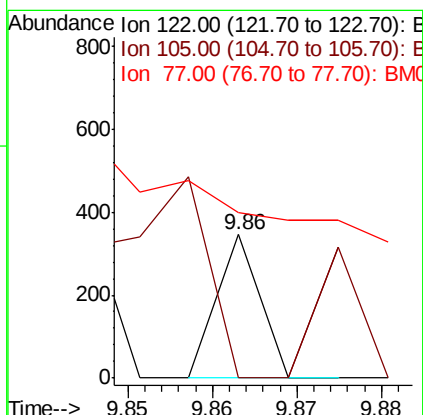

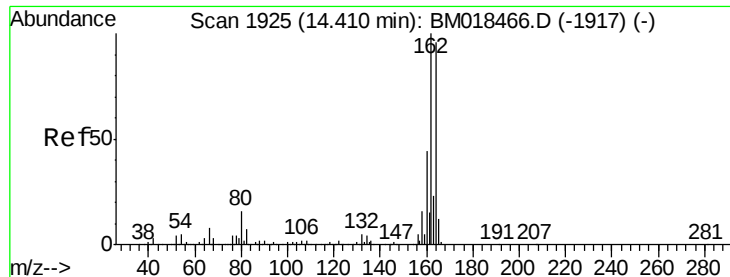

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.39 min Scan# 1922

Delta R.T. -0.02 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26

Instrument :

BNA\_M

ClientSampleId :

SW001-190114-01


Tgt Ion:164 Resp: 275696

Ion Ratio Lower Upper

164 100

162 105.5 83.0 124.4

160 45.6 37.1 55.7






Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

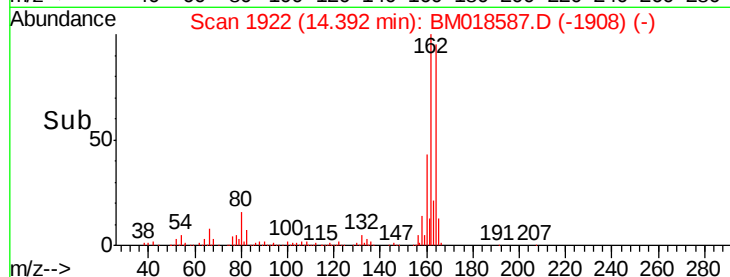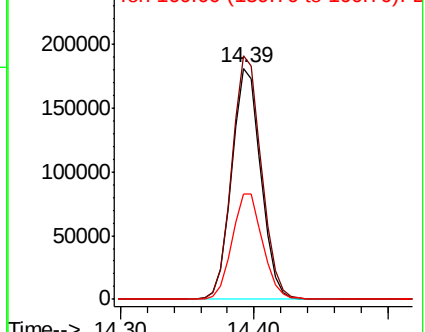

#42

2,4,6-Tribromophenol

Concen: 151.359 ng

RT: 15.89 min Scan# 2177

Delta R.T. -0.01 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26


Tgt Ion:330 Resp: 531329

Ion Ratio Lower Upper

330 100

332 97.4 77.6 116.4

141 38.3 31.7 47.5






Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



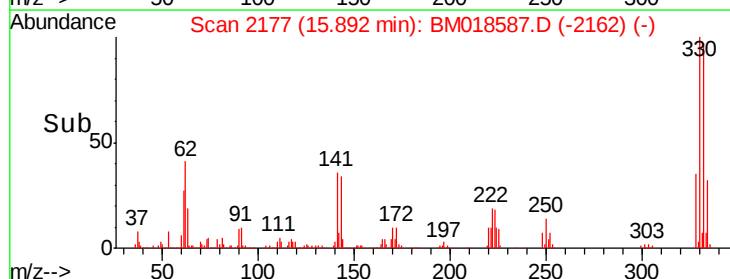
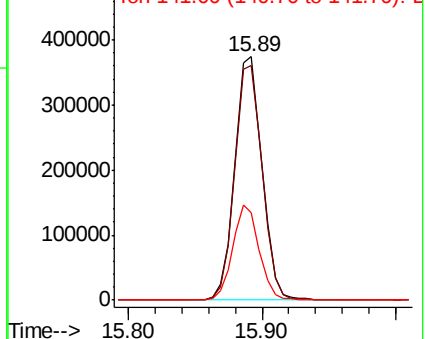


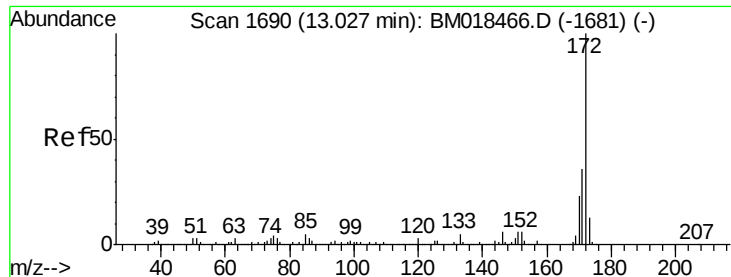

#45  
 2-Fluorobiphenyl  
 Concen: 80.867 ng  
 RT: 13.01 min Scan# 1687  
 Delta R.T. -0.01 min  
 Lab File: BM018587.D  
 Acq: 16 Jan 2019 17:26




Instrument :  
 BNA\_M  
 ClientSampleId :  
 SW001-190114-01


Tgt Ion:172 Resp: 1708590  
 Ion Ratio Lower Upper  
 172 100  
 171 35.0 28.2 42.4  
 170 22.7 18.9 28.3

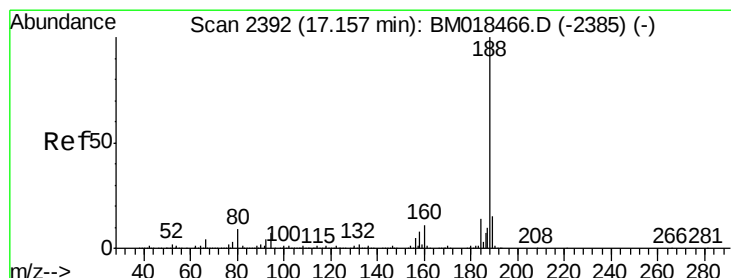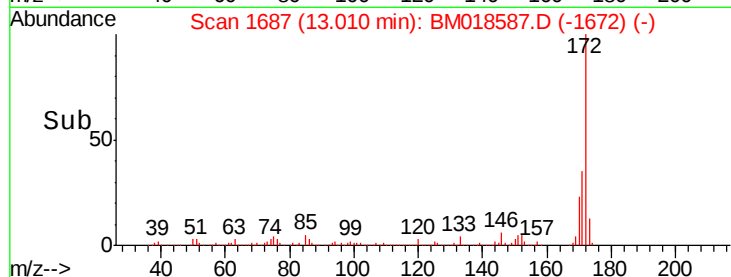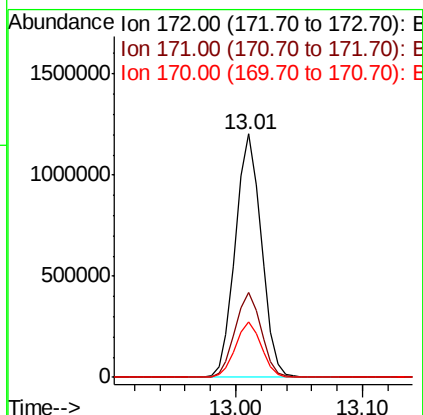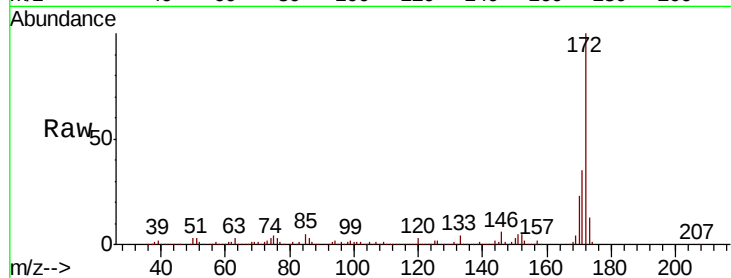

#64  
 Phenanthrene-d10  
 Concen: 20.000 ng  
 RT: 17.14 min Scan# 2390  
 Delta R.T. -0.01 min  
 Lab File: BM018587.D  
 Acq: 16 Jan 2019 17:26

Tgt Ion:188 Resp: 672337  
 Ion Ratio Lower Upper  
 188 100  
 94 7.4 7.1 10.7  
 80 8.2 7.6 11.4

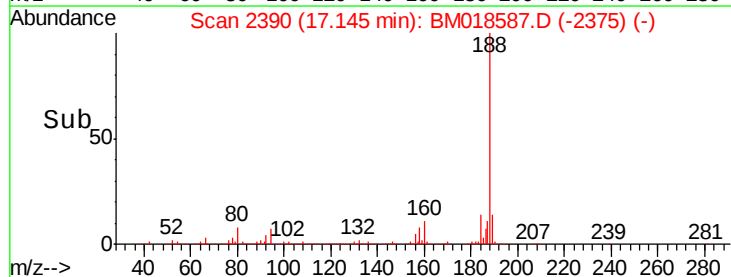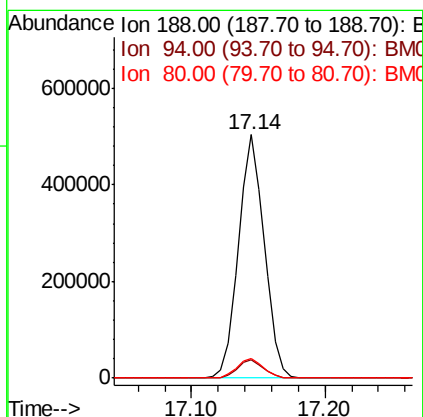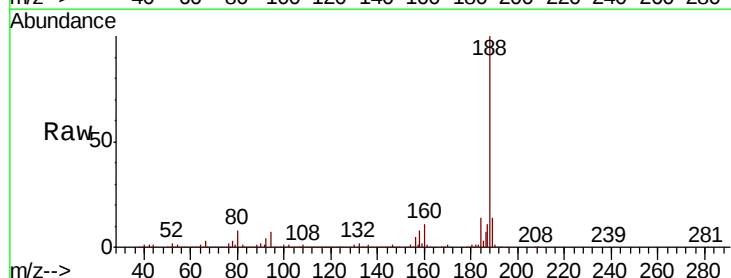

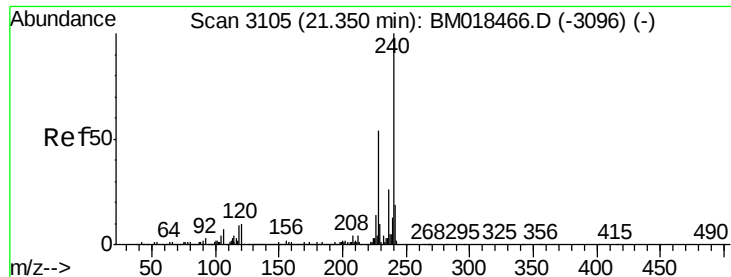

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.34 min Scan# 3103

Delta R.T. -0.01 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26

Instrument :

BNA\_M

ClientSampleId :

SW001-190114-01


Tgt Ion:240 Resp: 1004758

Ion Ratio Lower Upper

240 100

120 9.8 8.4 12.6




236 26.5 20.7 31.1

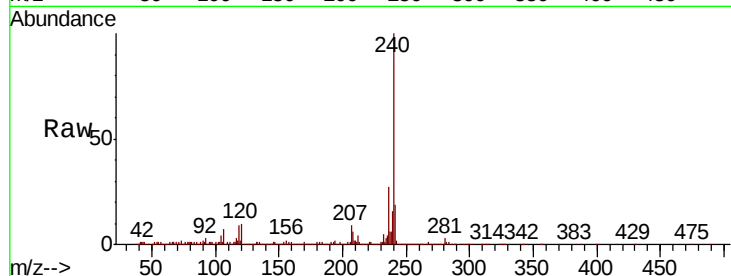

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

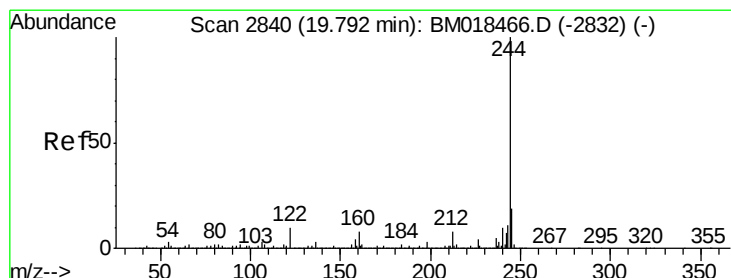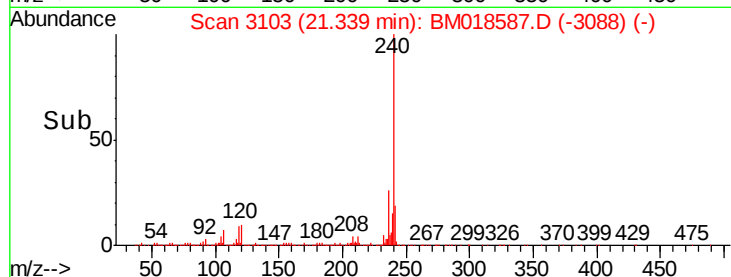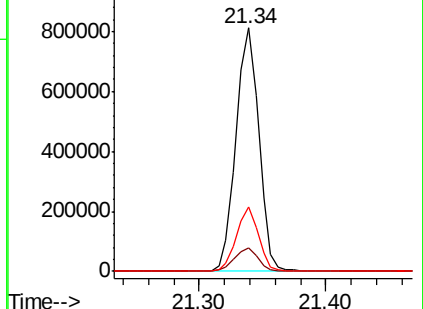

#79

Terphenyl-d14

Concen: 71.622 ng

RT: 19.77 min Scan# 2837

Delta R.T. -0.01 min

Lab File: BM018587.D

Acq: 16 Jan 2019 17:26


Tgt Ion:244 Resp: 3413752

Ion Ratio Lower Upper

244 100

212 7.6 5.9 8.9



122 9.9 9.0 13.4

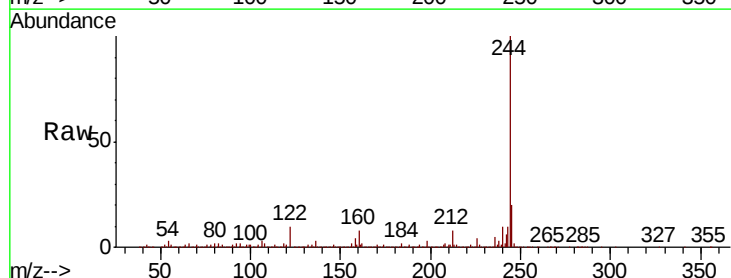


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

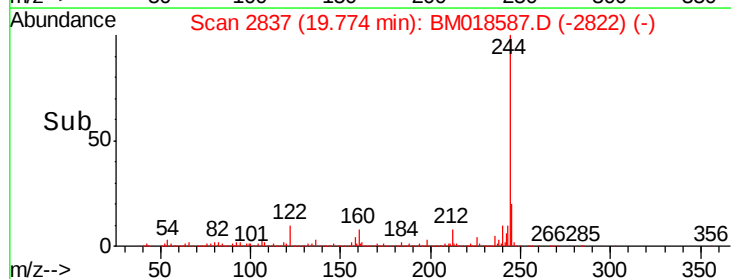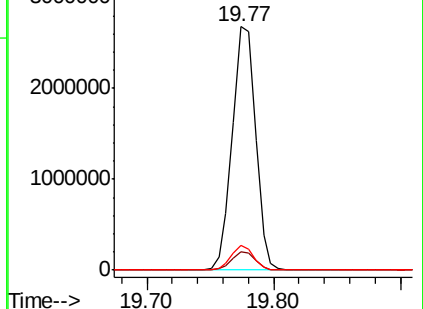

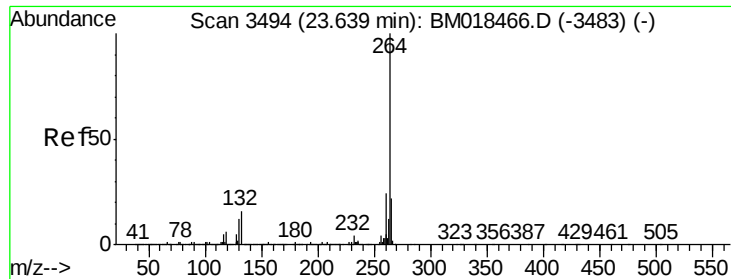

#87  
Perylene-d12  
Concen: 20.000 ng  
RT: 23.62 min Scan# 3490  
Delta R.T. -0.02 min  
Lab File: BM018587.D  
Acq: 16 Jan 2019 17:26

Instrument :  
BNA\_M  
ClientSampleId :  
SW001-190114-01

Tgt Ion: 264 Resp: 1266354  

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 264 | 100   |       |       |
| 260 | 23.5  | 18.9  | 28.3  |
| 265 | 21.7  | 16.8  | 25.2  |

