

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM011619\
 Data File : BM018601.D
 Acq On : 17 Jan 2019 03:11
 Operator : JU/SJ
 Sample : K1147-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-1

Quant Time: Jan 17 05:52:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 10 05:57:41 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	353923	20.00	ng	-0.02
21) Naphthalene-d8	10.53	136	1429247	20.00	ng	-0.02
39) Acenaphthene-d10	14.39	164	802407	20.00	ng	-0.02
64) Phenanthrene-d10	17.14	188	1849884	20.00	ng	-0.01
76) Chrysene-d12	21.33	240	1767548	20.00	ng	-0.02
87) Perylene-d12	23.61	264	1373737	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	2451479	127.90	ng	-0.01
7) Phenol-d6	6.93	99	2769791	113.77	ng	0.00
23) Nitrobenzene-d5	8.92	82	2265867	91.90	ng	0.00
42) 2,4,6-Tribromophenol	15.89	330	1539654	150.70	ng	-0.01
45) 2-Fluorobiphenyl	13.01	172	5578965	90.72	ng	-0.01
79) Terphenyl-d14	19.78	244	8883289	105.94	ng	0.00
Target Compounds						
32) Benzoic acid	9.87	122	136	6.512	ng	Qvalue # 30


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM011619\
Data File : BM018601.D
Acq On : 17 Jan 2019 03:11
Operator : JU/SJ
Sample : K1147-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-1

Quant Time: Jan 17 05:52:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

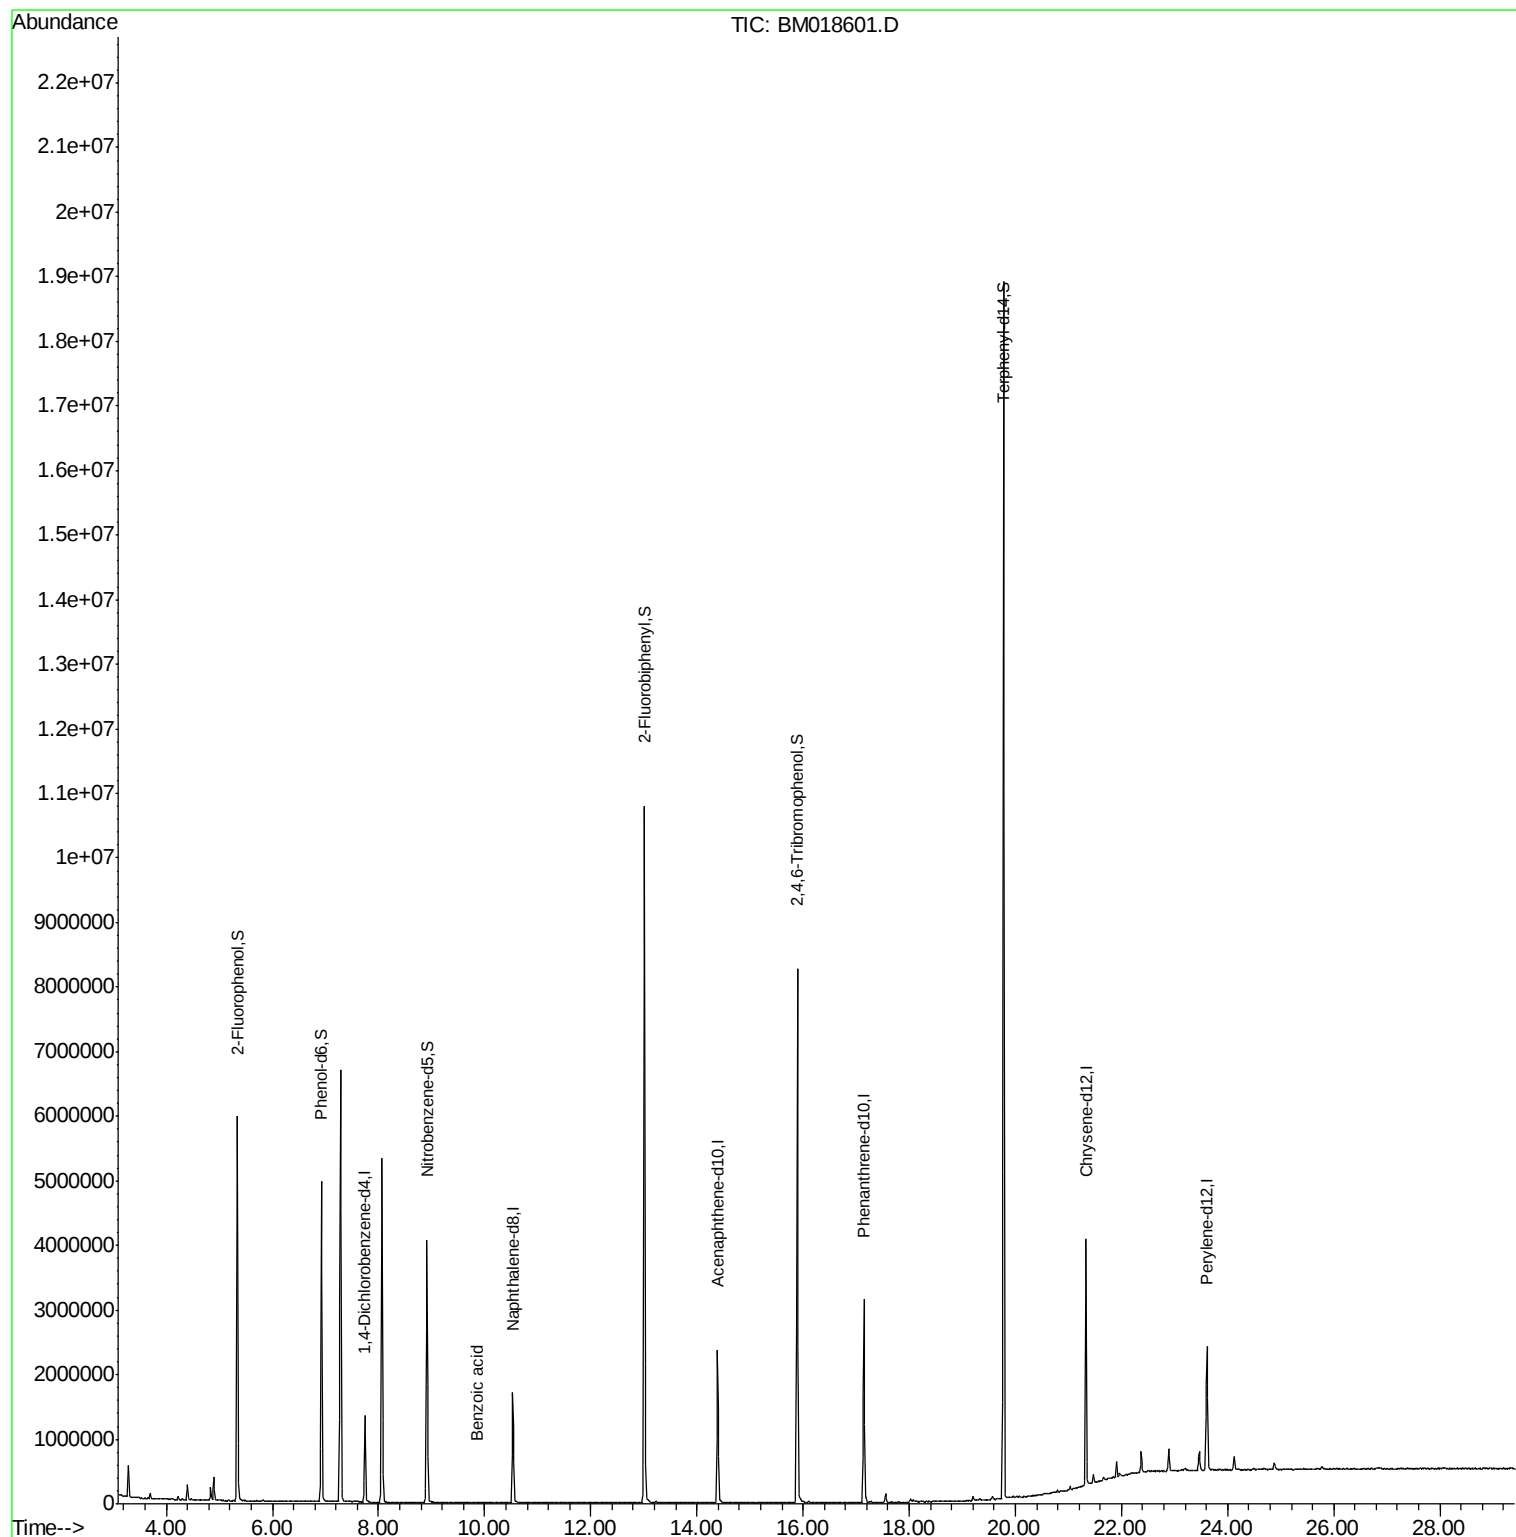

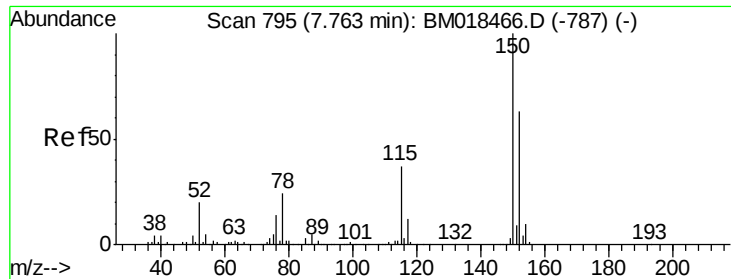


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.75 min Scan# 792
Delta R.T. -0.02 min
Lab File: BM018601.D
Acq: 17 Jan 2019 03:11

Instrument :
BNA_M
ClientSampleId :
TP-1

Tgt Ion:152 Resp: 353923
Ion Ratio Lower Upper
152 100
150 155.7 126.9 190.3
115 58.0 45.5 68.3

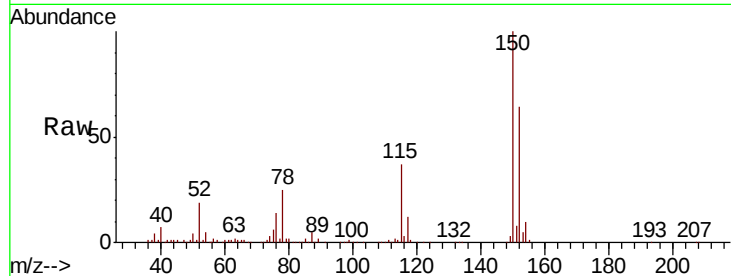


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

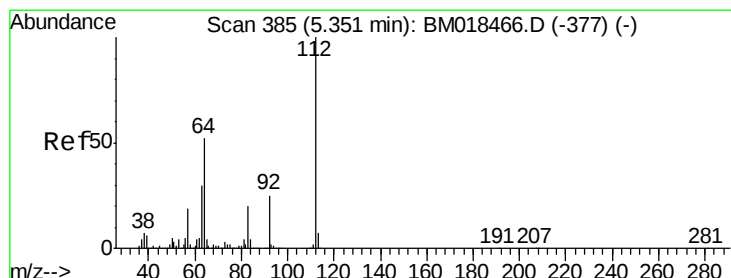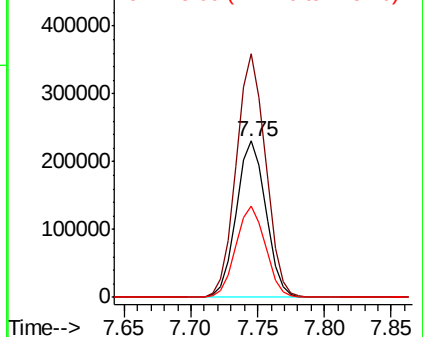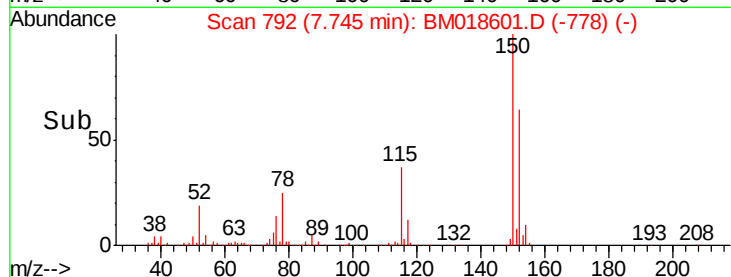



#5


2-Fluorophenol
Concen: 127.899 ng
RT: 5.34 min Scan# 383
Delta R.T. -0.01 min
Lab File: BM018601.D
Acq: 17 Jan 2019 03:11

Tgt Ion:112 Resp: 2451479
Ion Ratio Lower Upper
112 100
64 52.9 46.5 69.7
63 29.7 25.2 37.8

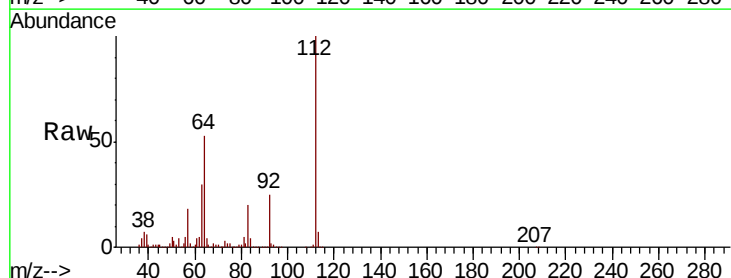

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

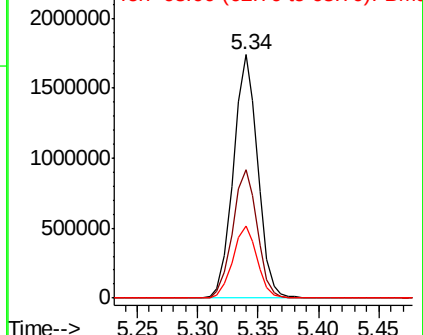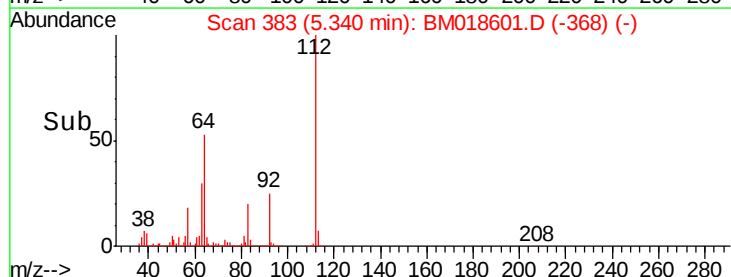

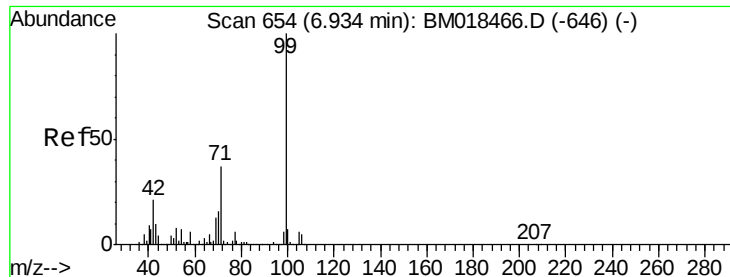

#7

Phenol-d6

Concen: 113.774 ng

RT: 6.93 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM018601.D

Acq: 17 Jan 2019 03:11

Instrument :

BNA_M

ClientSampleId :

TP-1


Tgt Ion: 99 Resp: 2769791

Ion Ratio Lower Upper

99 100

42 19.4 17.3 25.9




71 35.8 28.0 42.0

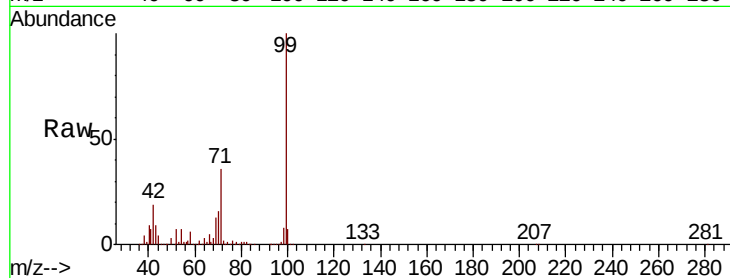

Abundance Ion 99.00 (98.70 to 99.70): BM018466.D (-646) (-)

Ion 42.00 (41.70 to 42.70): BM018466.D (-646) (-)

Ion 71.00 (70.70 to 71.70): BM018466.D (-646) (-)

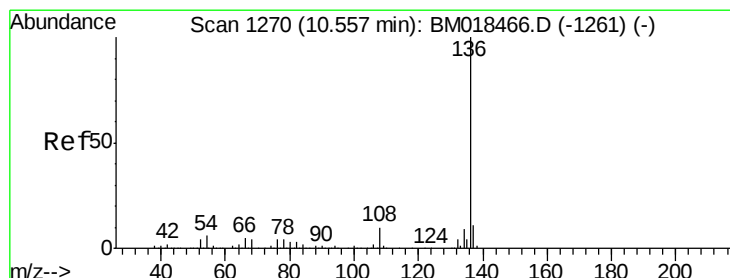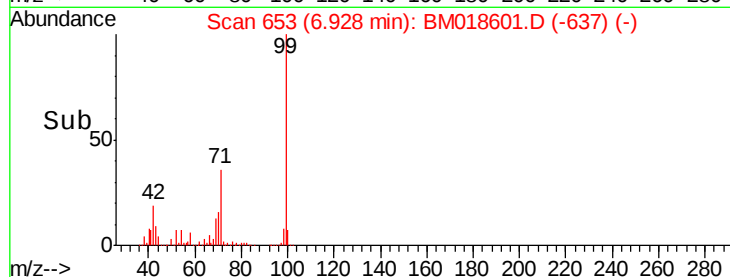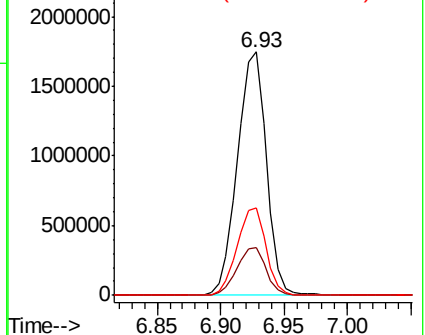

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.53 min Scan# 1266

Delta R.T. -0.02 min

Lab File: BM018601.D

Acq: 17 Jan 2019 03:11

Tgt Ion: 136 Resp: 1429247


Ion Ratio Lower Upper

136 100

137 10.8 8.5 12.7

54 6.4 6.0 9.0

68 4.6 4.5 6.7


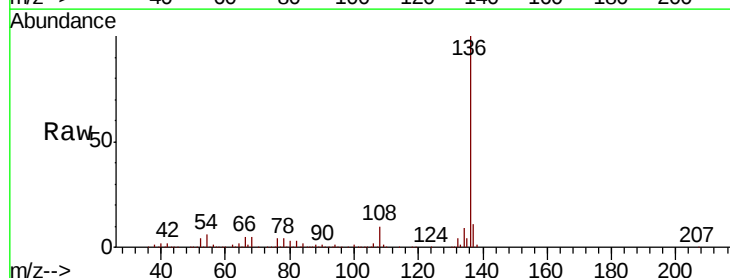


Abundance Ion 136.00 (135.70 to 136.70): BM018466.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM018466.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM018466.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM018466.D (-1261) (-)



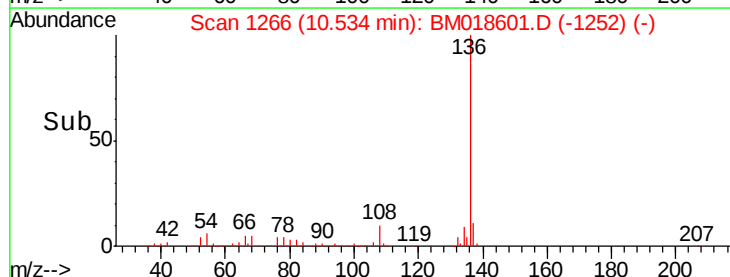
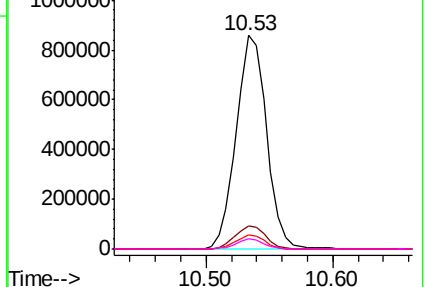




#23
 Nitrobenzene-d5
 Concen: 91.905 ng
 RT: 8.92 min Scan# 991
 Delta R.T. -0.01 min
 Lab File: BM018601.D
 Acq: 17 Jan 2019 03:11




Instrument :
 BNA_M
 ClientSampleID :
 TP-1

Tgt Ion: 82 Resp: 2265867
 Ion Ratio Lower Upper
 82 100
 128 47.0 36.3 54.5
 54 48.9 41.7 62.5

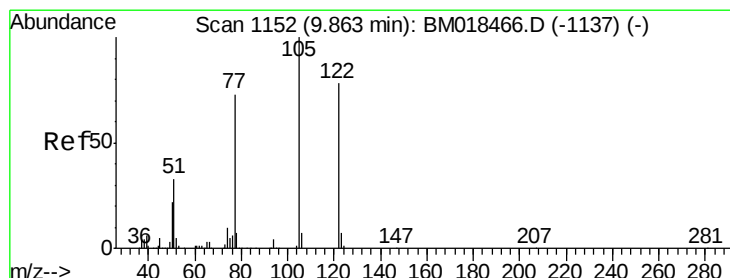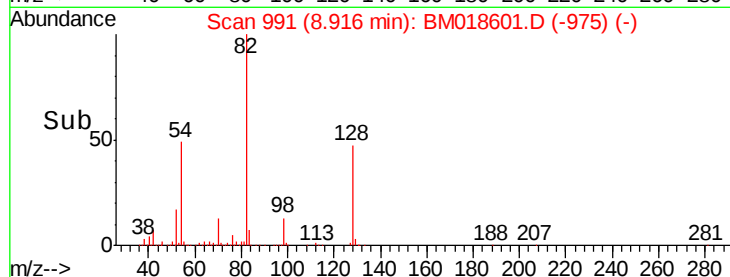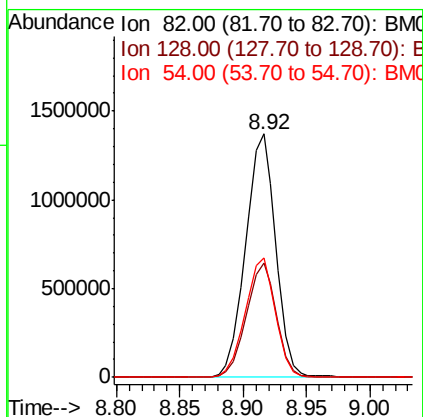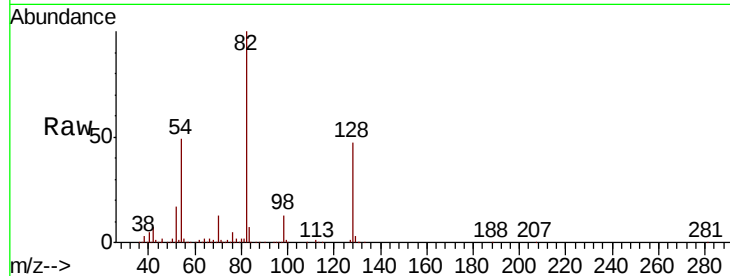

#32
 Benzoic acid
 Concen: 6.512 ng
 RT: 9.87 min Scan# 1153
 Delta R.T. -0.04 min
 Lab File: BM018601.D
 Acq: 17 Jan 2019 03:11

Tgt Ion: 122 Resp: 136
 Ion Ratio Lower Upper
 122 100
 105 0.0 100.4 140.4#
 77 111.2 71.7 111.7

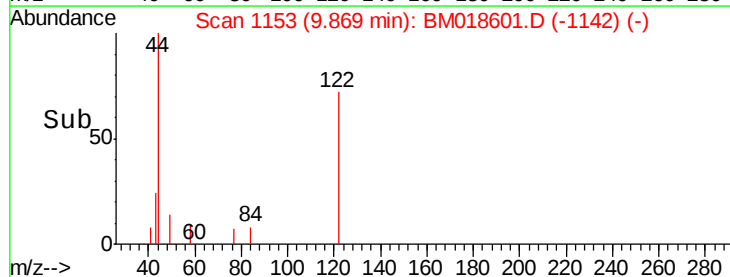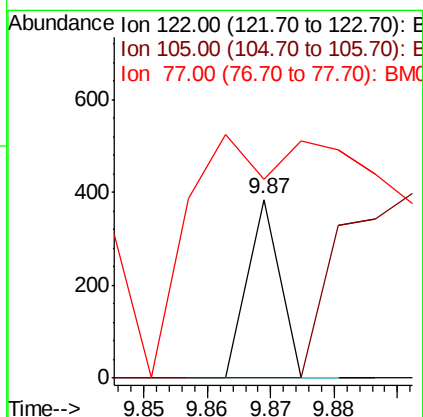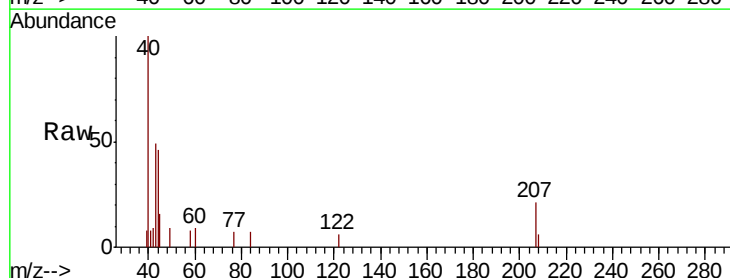



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.39 min Scan# 1922

Delta R.T. -0.02 min

Lab File: BM018601.D

Acq: 17 Jan 2019 03:11

Instrument :

BNA_M

ClientSampleId :

TP-1


Tgt Ion:164 Resp: 802407

Ion Ratio Lower Upper

164 100

162 105.3 83.0 124.4




160 46.7 37.1 55.7

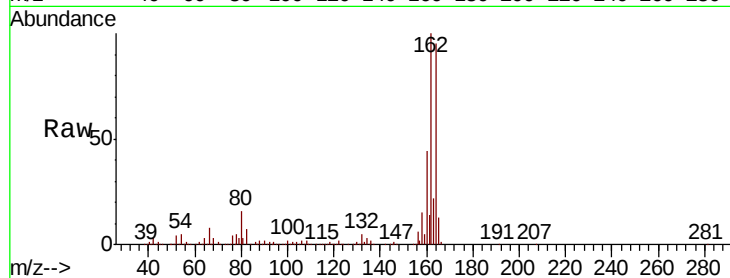

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

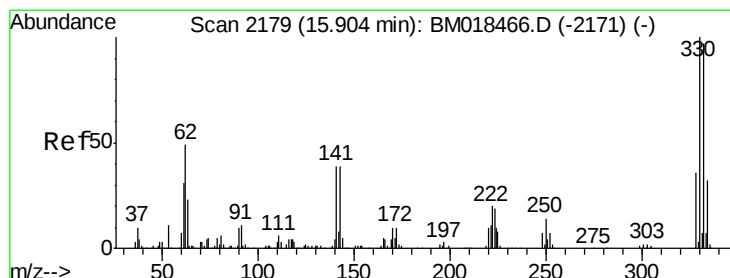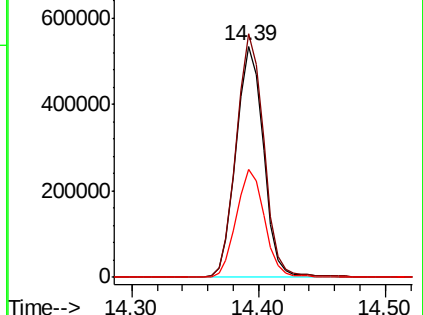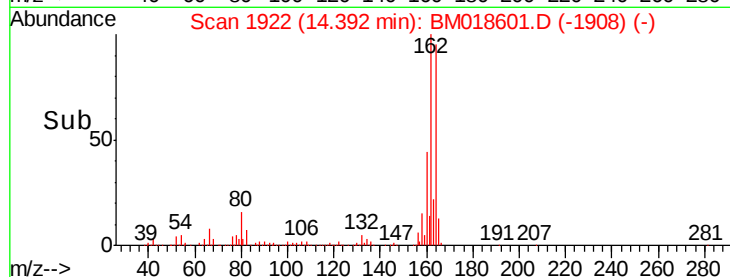

#42

2,4,6-Tribromophenol

Concen: 150.697 ng

RT: 15.89 min Scan# 2177

Delta R.T. -0.01 min

Lab File: BM018601.D

Acq: 17 Jan 2019 03:11


Tgt Ion:330 Resp: 1539654

Ion Ratio Lower Upper

330 100

332 96.7 77.6 116.4



141 37.3 31.7 47.5

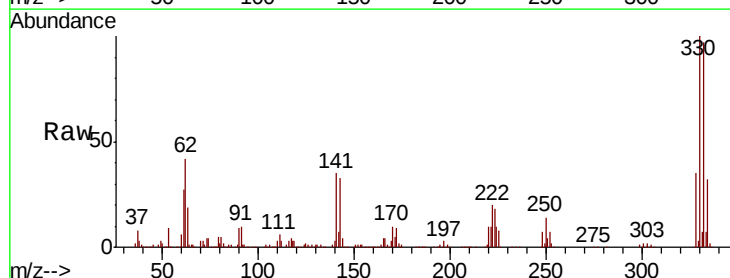


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

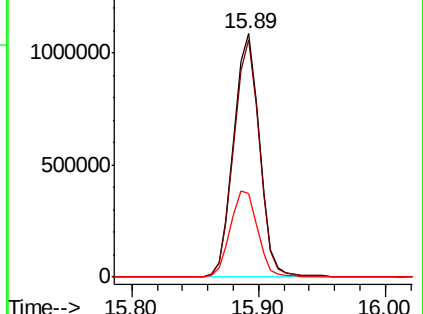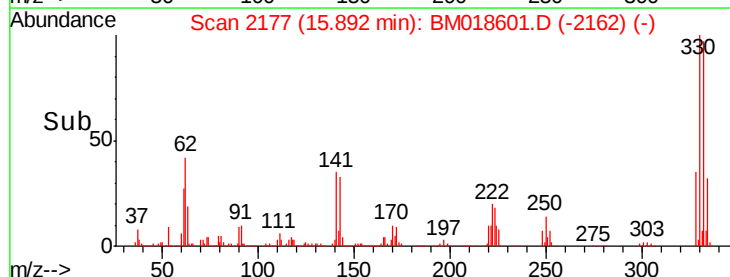


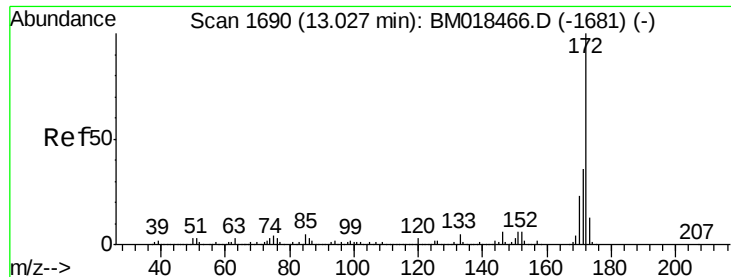




#45
2-Fluorobiphenyl
Concen: 90.724 ng
RT: 13.01 min Scan# 1687
Delta R.T. -0.01 min
Lab File: BM018601.D
Acq: 17 Jan 2019 03:11

Instrument :
BNA_M
ClientSampleId :
TP-1

Tgt Ion:172 Resp: 5578965
Ion Ratio Lower Upper
172 100
171 35.3 28.2 42.4
170 23.4 18.9 28.3

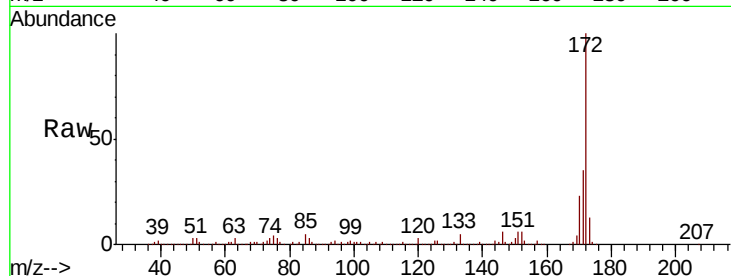


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

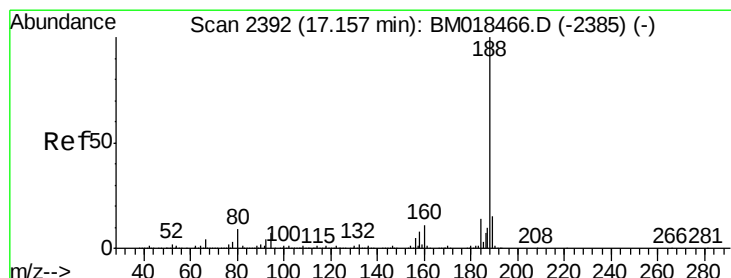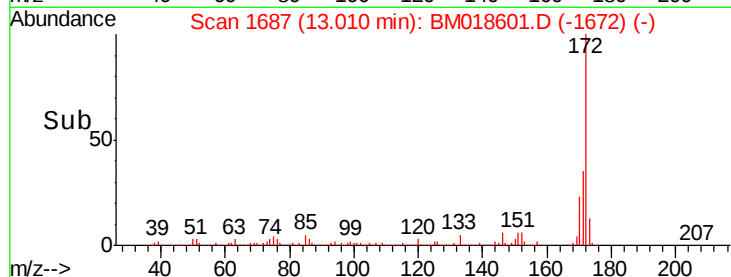
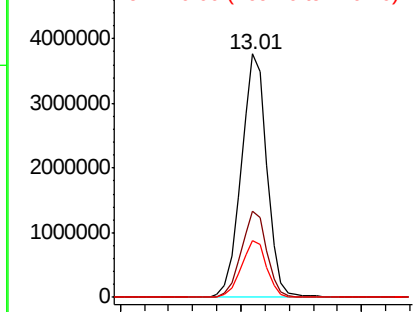



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.14 min Scan# 2390
Delta R.T. -0.01 min
Lab File: BM018601.D
Acq: 17 Jan 2019 03:11

Tgt Ion:188 Resp: 1849884
Ion Ratio Lower Upper
188 100
94 7.3 7.1 10.7
80 8.1 7.6 11.4

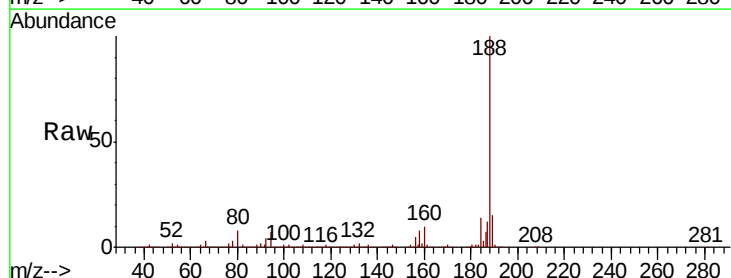

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0



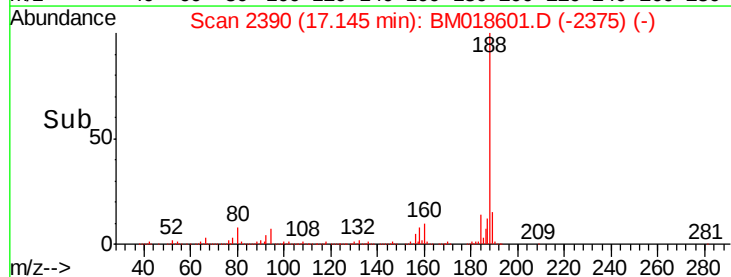
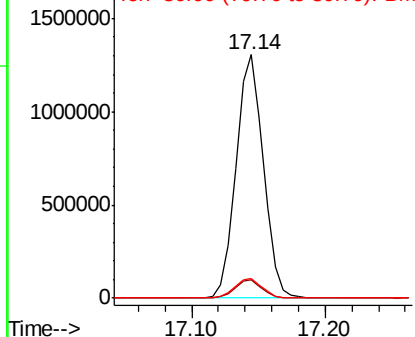


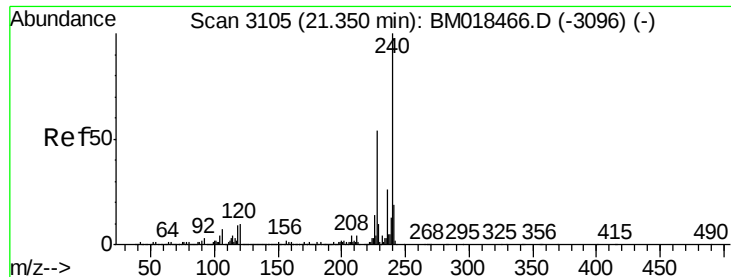

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.33 min Scan# 3102
Delta R.T. -0.02 min
Lab File: BM018601.D
Acq: 17 Jan 2019 03:11




Instrument :
BNA_M
ClientSampleId :
TP-1


Tgt Ion:240 Resp: 1767548
Ion Ratio Lower Upper
240 100
120 9.3 8.4 12.6
236 25.4 20.7 31.1

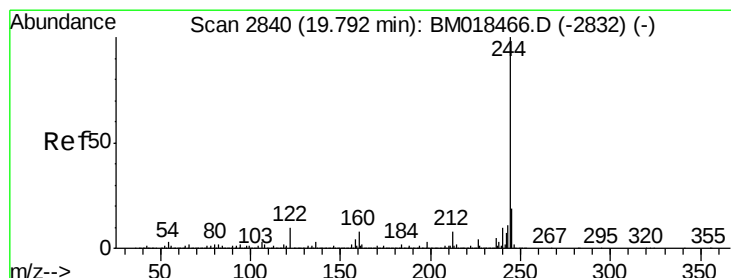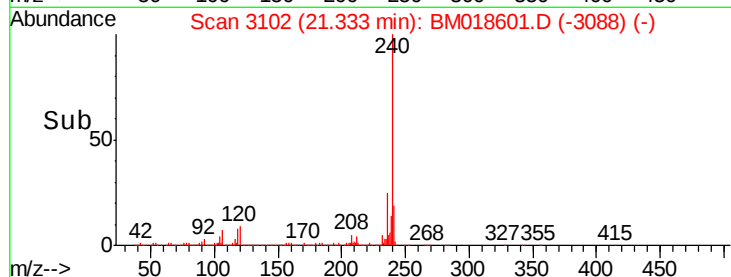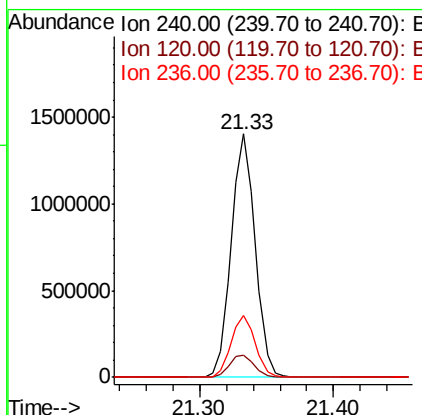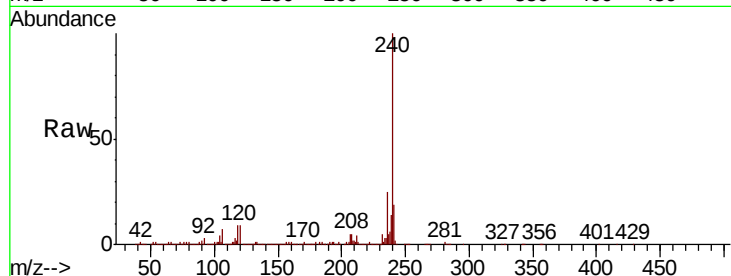

#79
Terphenyl-d14
Concen: 105.945 ng
RT: 19.78 min Scan# 2838
Delta R.T. -0.01 min
Lab File: BM018601.D
Acq: 17 Jan 2019 03:11

Tgt Ion:244 Resp: 8883289
Ion Ratio Lower Upper
244 100
212 8.0 5.9 8.9
122 9.5 9.0 13.4

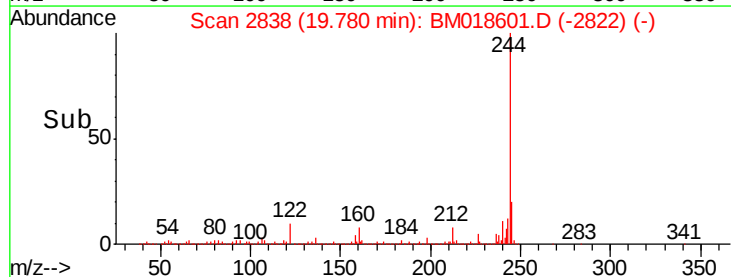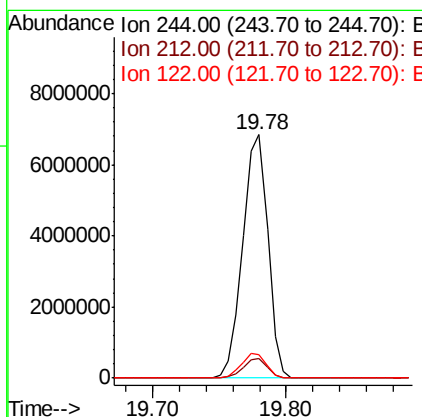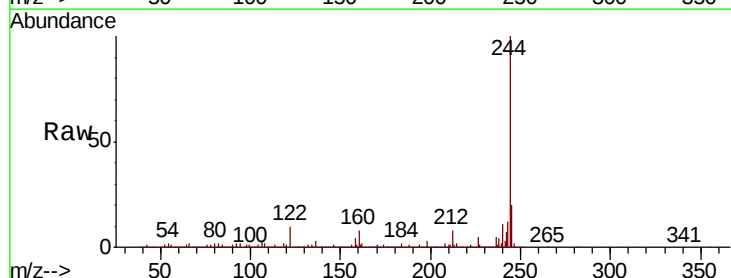

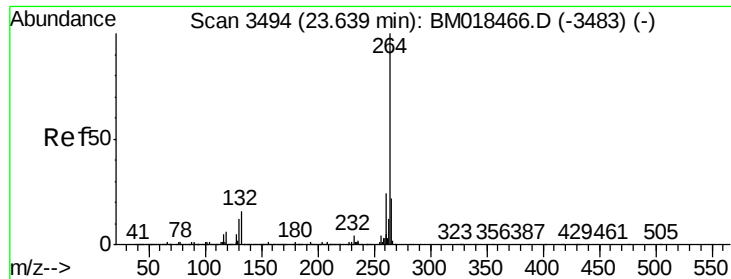

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.61 min Scan# 3489

Delta R.T. -0.02 min

Lab File: BM018601.D

Acq: 17 Jan 2019 03:11

Instrument :

BNA_M

ClientSampleId :

TP-1

Tgt Ion:264 Resp: 1373737

Ion Ratio Lower Upper

264 100

260 23.8 18.9 28.3

265 21.9 16.8 25.2

