
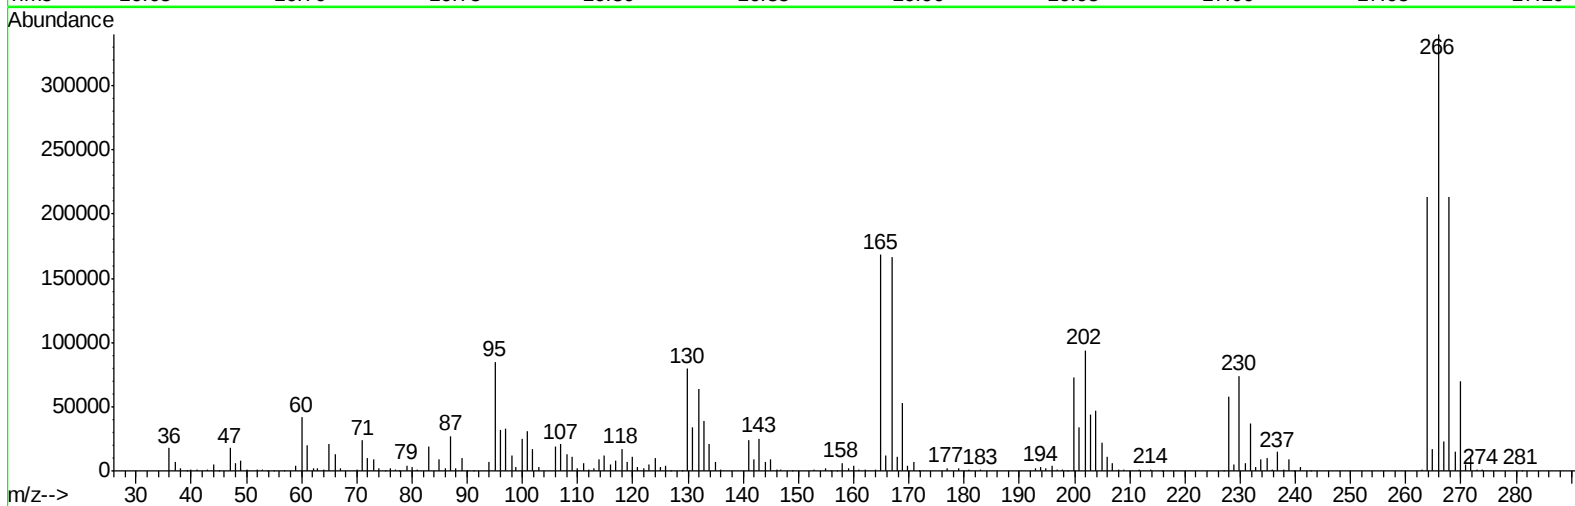


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011619\
Data File : BM018577.D
Acq On : 16 Jan 2019 10:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 08:12:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

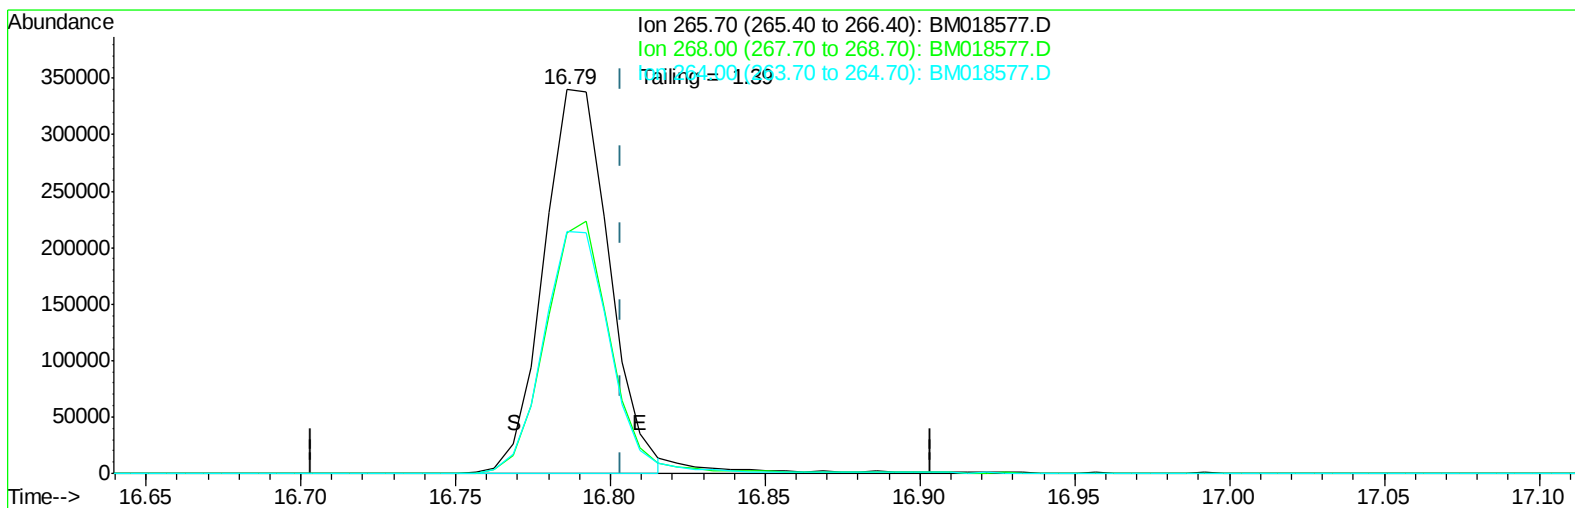

TIC: BM018577.D

(70) Pentachlorophenol (C)



16.786min (-0.017) 96700.05ng

response 510151

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.81
264.00	62.60	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011619\
Data File : BM018577.D
Acq On : 16 Jan 2019 10:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 08:12:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

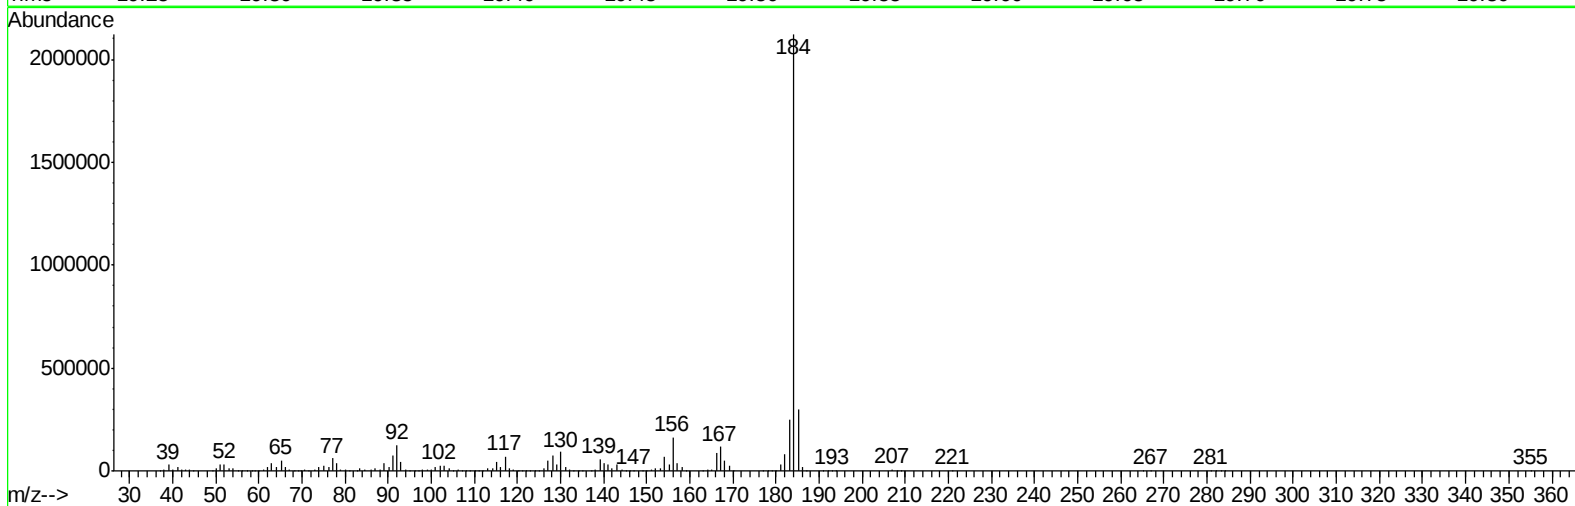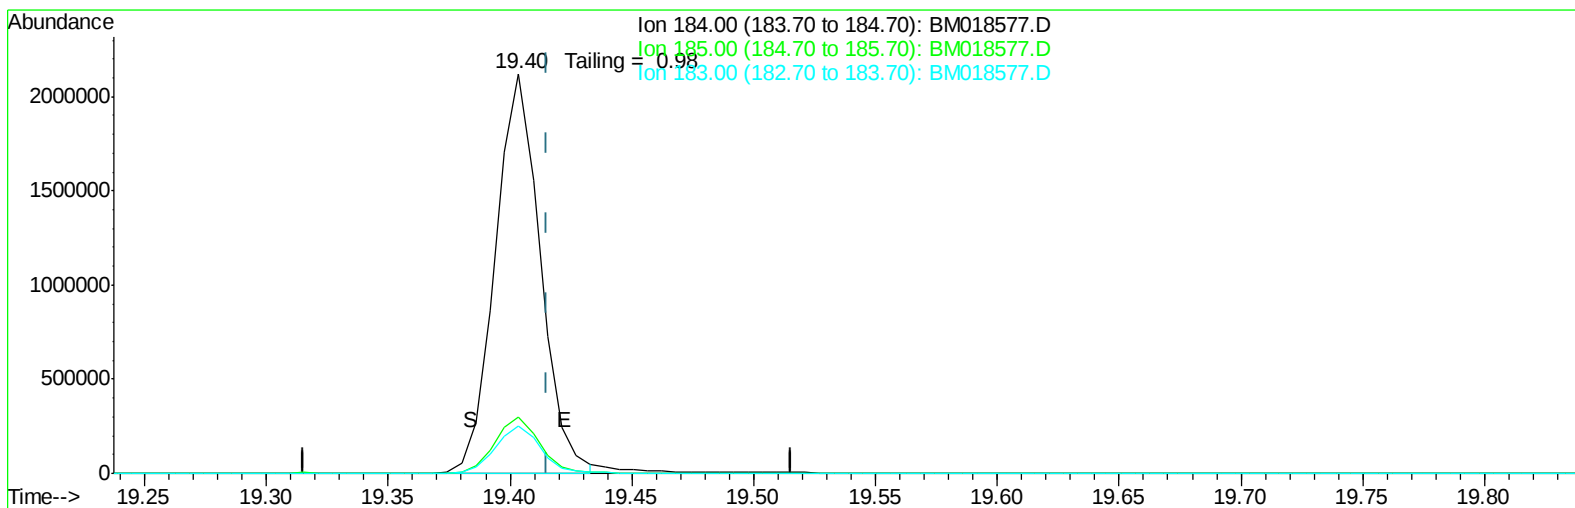

TIC: BM018577.D

(77) Benzidine

19.404min (-0.012) 90395.92ng

response 2758761

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.08
183.00	11.90	11.78
0.00	0.00	0.00