
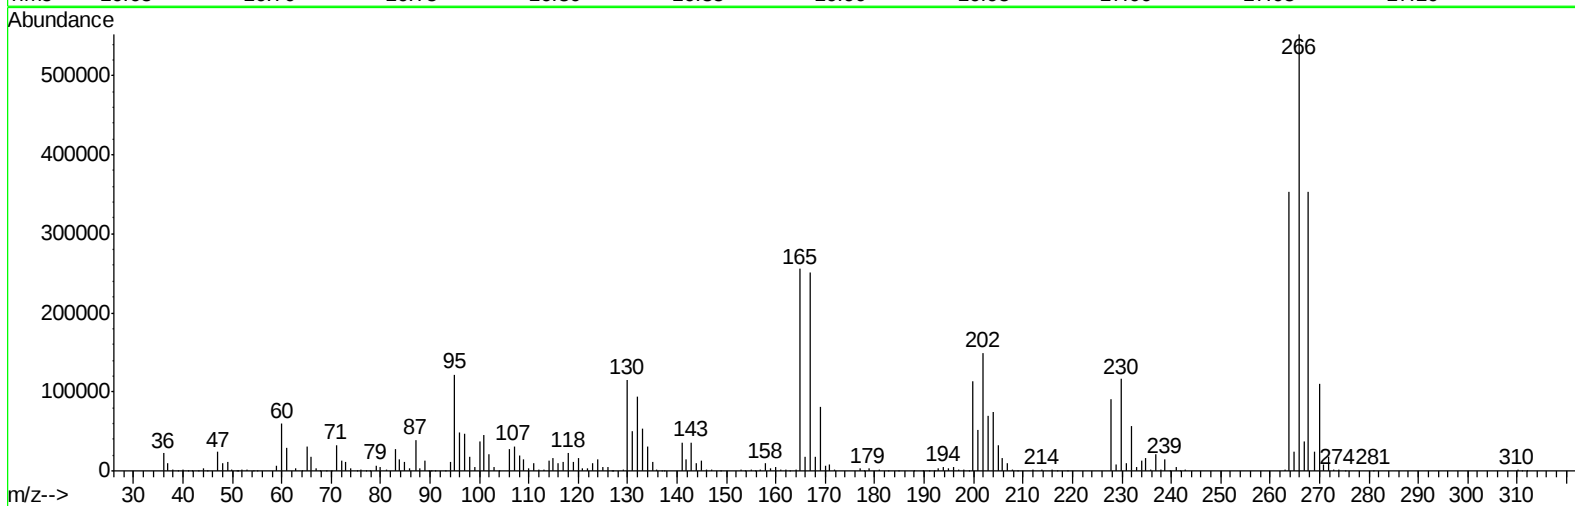


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011619\
Data File : BM018596.D
Acq On : 16 Jan 2019 23:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 08:22:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

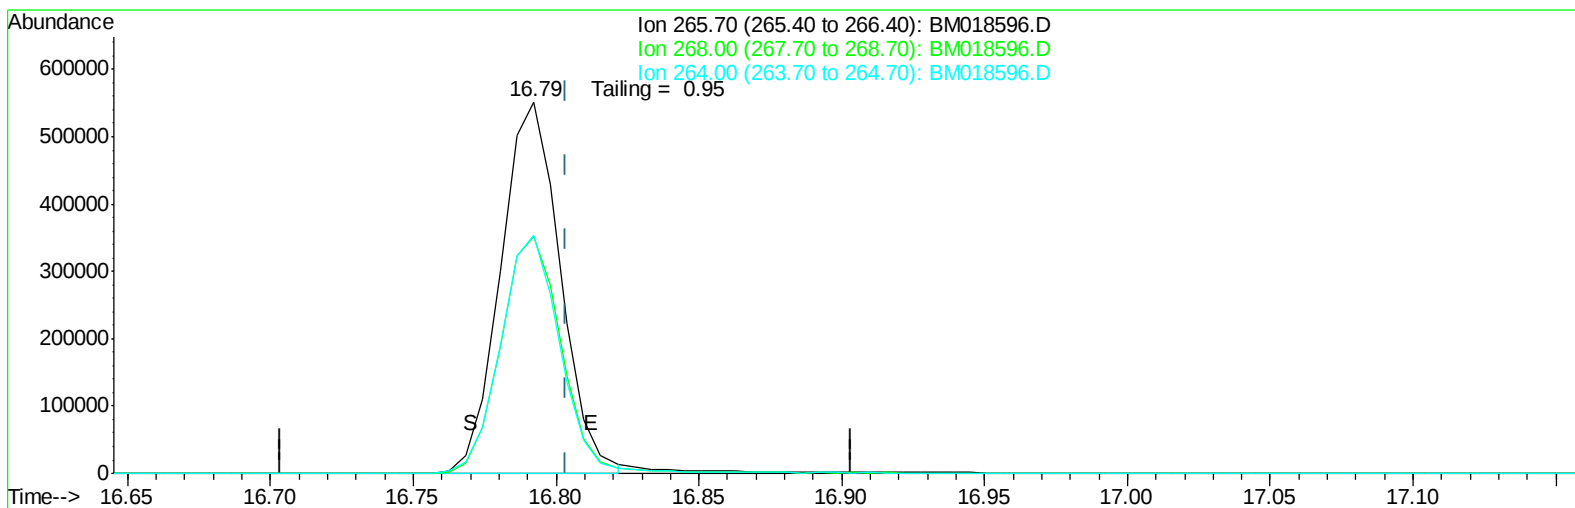

TIC: BM018596.D

(70) Pentachlorophenol (C)



16.792min (-0.011) 88870.23ng

response 812274

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.84
264.00	62.60	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011619\
Data File : BM018596.D
Acq On : 16 Jan 2019 23:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 08:22:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

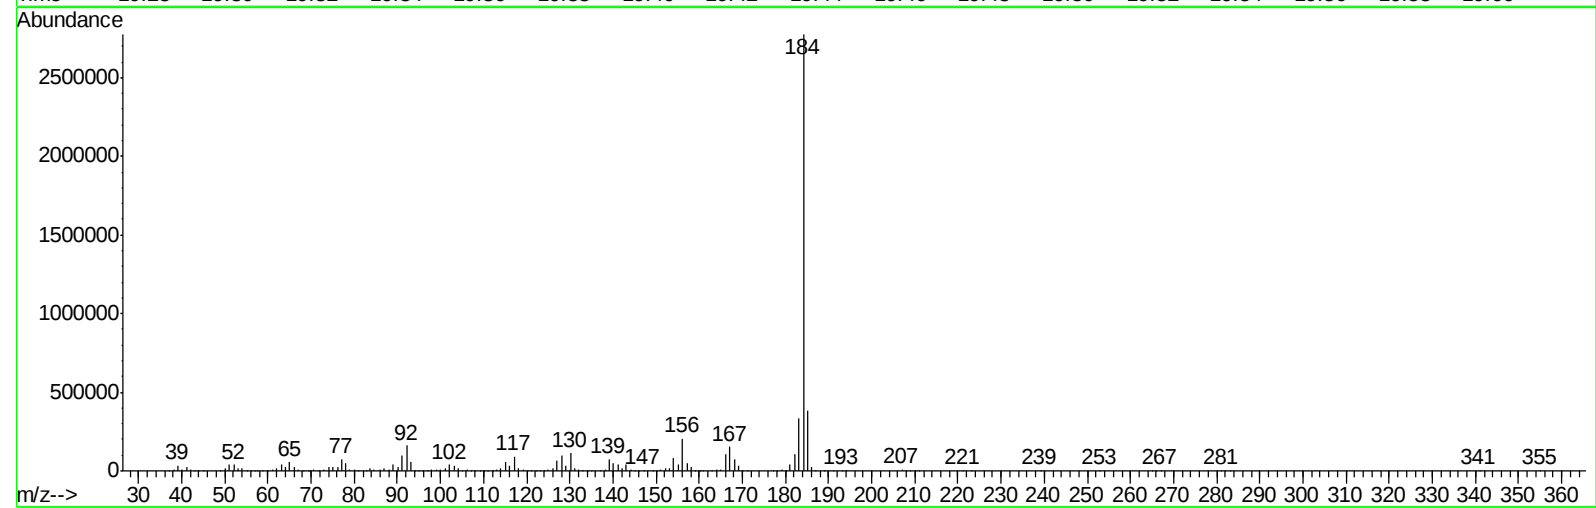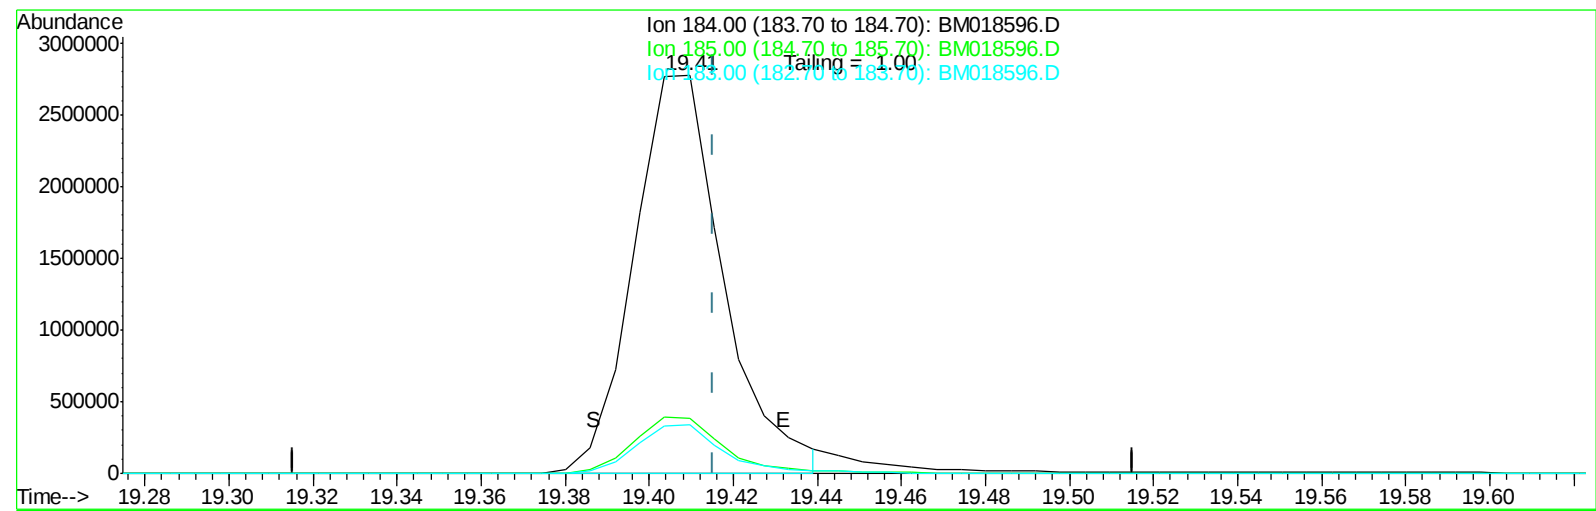

TIC: BM018596.D

(77) Benzidine

19.410min (-0.006) 35045.74ng

response 4237523

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.86
183.00	11.90	12.09
0.00	0.00	0.00