


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011619\  
 Data File : BM018577.D  
 Acq On : 16 Jan 2019 10:44  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM010919.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jan 10 05:57:41 2019

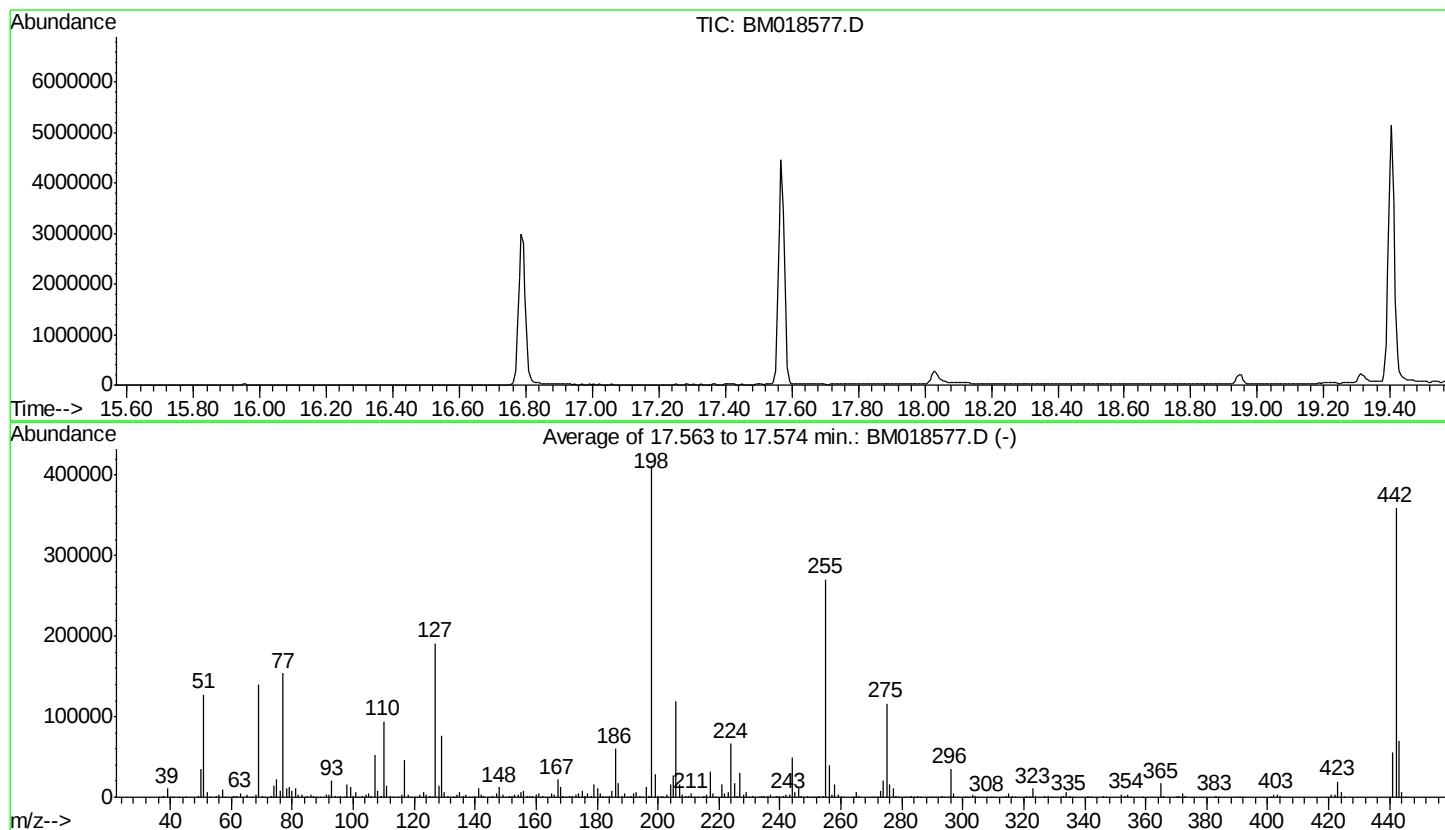

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 30.9      | 127272  | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 2791    | PASS             |
| 69          | 198          | 0.00         | 100          | 34.0      | 139740  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 903     | PASS             |
| 127         | 198          | 10           | 80           | 46.5      | 191424  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 2173    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 411584  | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 28829   | PASS             |
| 275         | 198          | 10           | 60           | 28.3      | 116421  | PASS             |
| 365         | 198          | 1            | 100          | 4.2       | 17279   | PASS             |
| 441         | 198          | 0.01         | 100          | 13.4      | 55170   | PASS             |
| 442         | 198          | 50           | 100          | 87.3      | 359360  | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 70469   | PASS             |