


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011619\
 Data File : BM018596.D
 Acq On : 16 Jan 2019 23:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

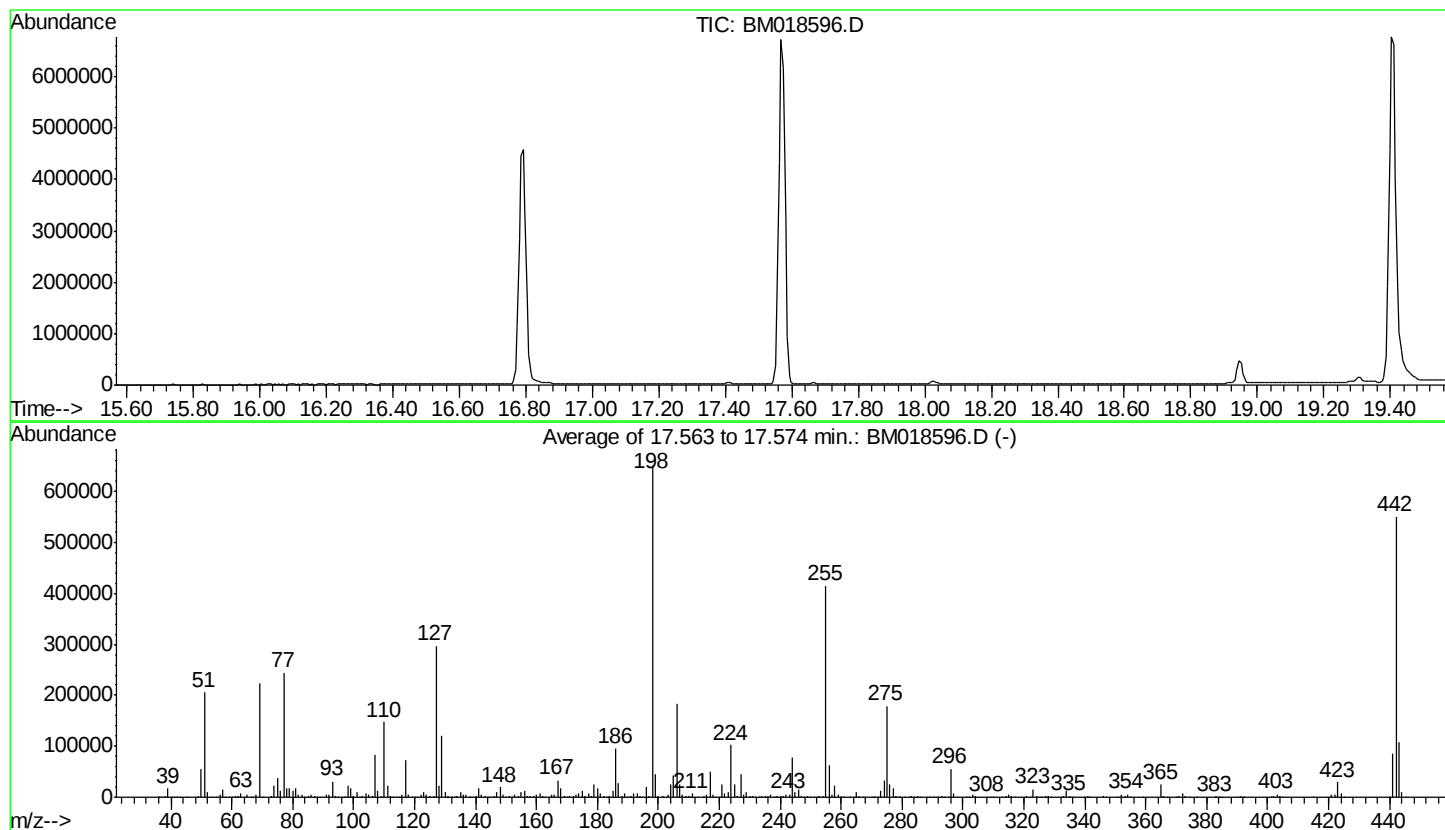

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	205909	PASS
68	69	0.00	2	1.8	3937	PASS
69	198	0.00	100	34.3	223030	PASS
70	69	0.00	2	0.5	1207	PASS
127	198	10	80	45.7	297578	PASS
197	198	0.00	2	0.6	3709	PASS
198	198	100	100	100.0	651008	PASS
199	198	5	9	6.9	44704	PASS
275	198	10	60	27.5	178893	PASS
365	198	1	100	3.9	25143	PASS
441	198	0.01	100	13.0	84754	PASS
442	198	50	100	84.6	551061	PASS
443	442	15	24	19.7	108738	PASS