

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011620\
 Data File : BM024489.D
 Acq On : 16 Jan 2020 11:26
 Operator : JU
 Sample : L1121-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GASJ0

Quant Time: Jan 16 12:11:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 16 01:52:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	146099	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	647860	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	504045	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	1195157	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1276751	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1468233	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	17741	5.93	ng/uL	0.00
5) Phenol-d5	6.65	99	82015	7.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	158331	26.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	207849	22.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	142902	14.31	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	133506	29.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	151088	30.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	279349	25.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	72182	5.85	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1190059	30.13	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1324376	29.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	42477	6.44	ng/ul	0.00
58) Fluorene-d10	15.11	176	1041379	29.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	183511	26.90	ng/ul	0.00
71) Anthracene-d10	16.96	188	1881606	33.86	ng/ul	0.00
79) Pyrene-d10	19.26	212	2295157	33.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2604637	34.20	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.57	163	69550	1.732	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011620\
Data File : BM024489.D
Acq On : 16 Jan 2020 11:26
Operator : JU
Sample : L1121-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASJ0

Quant Time: Jan 16 12:11:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 16 01:52:07 2020
Response via : Initial Calibration

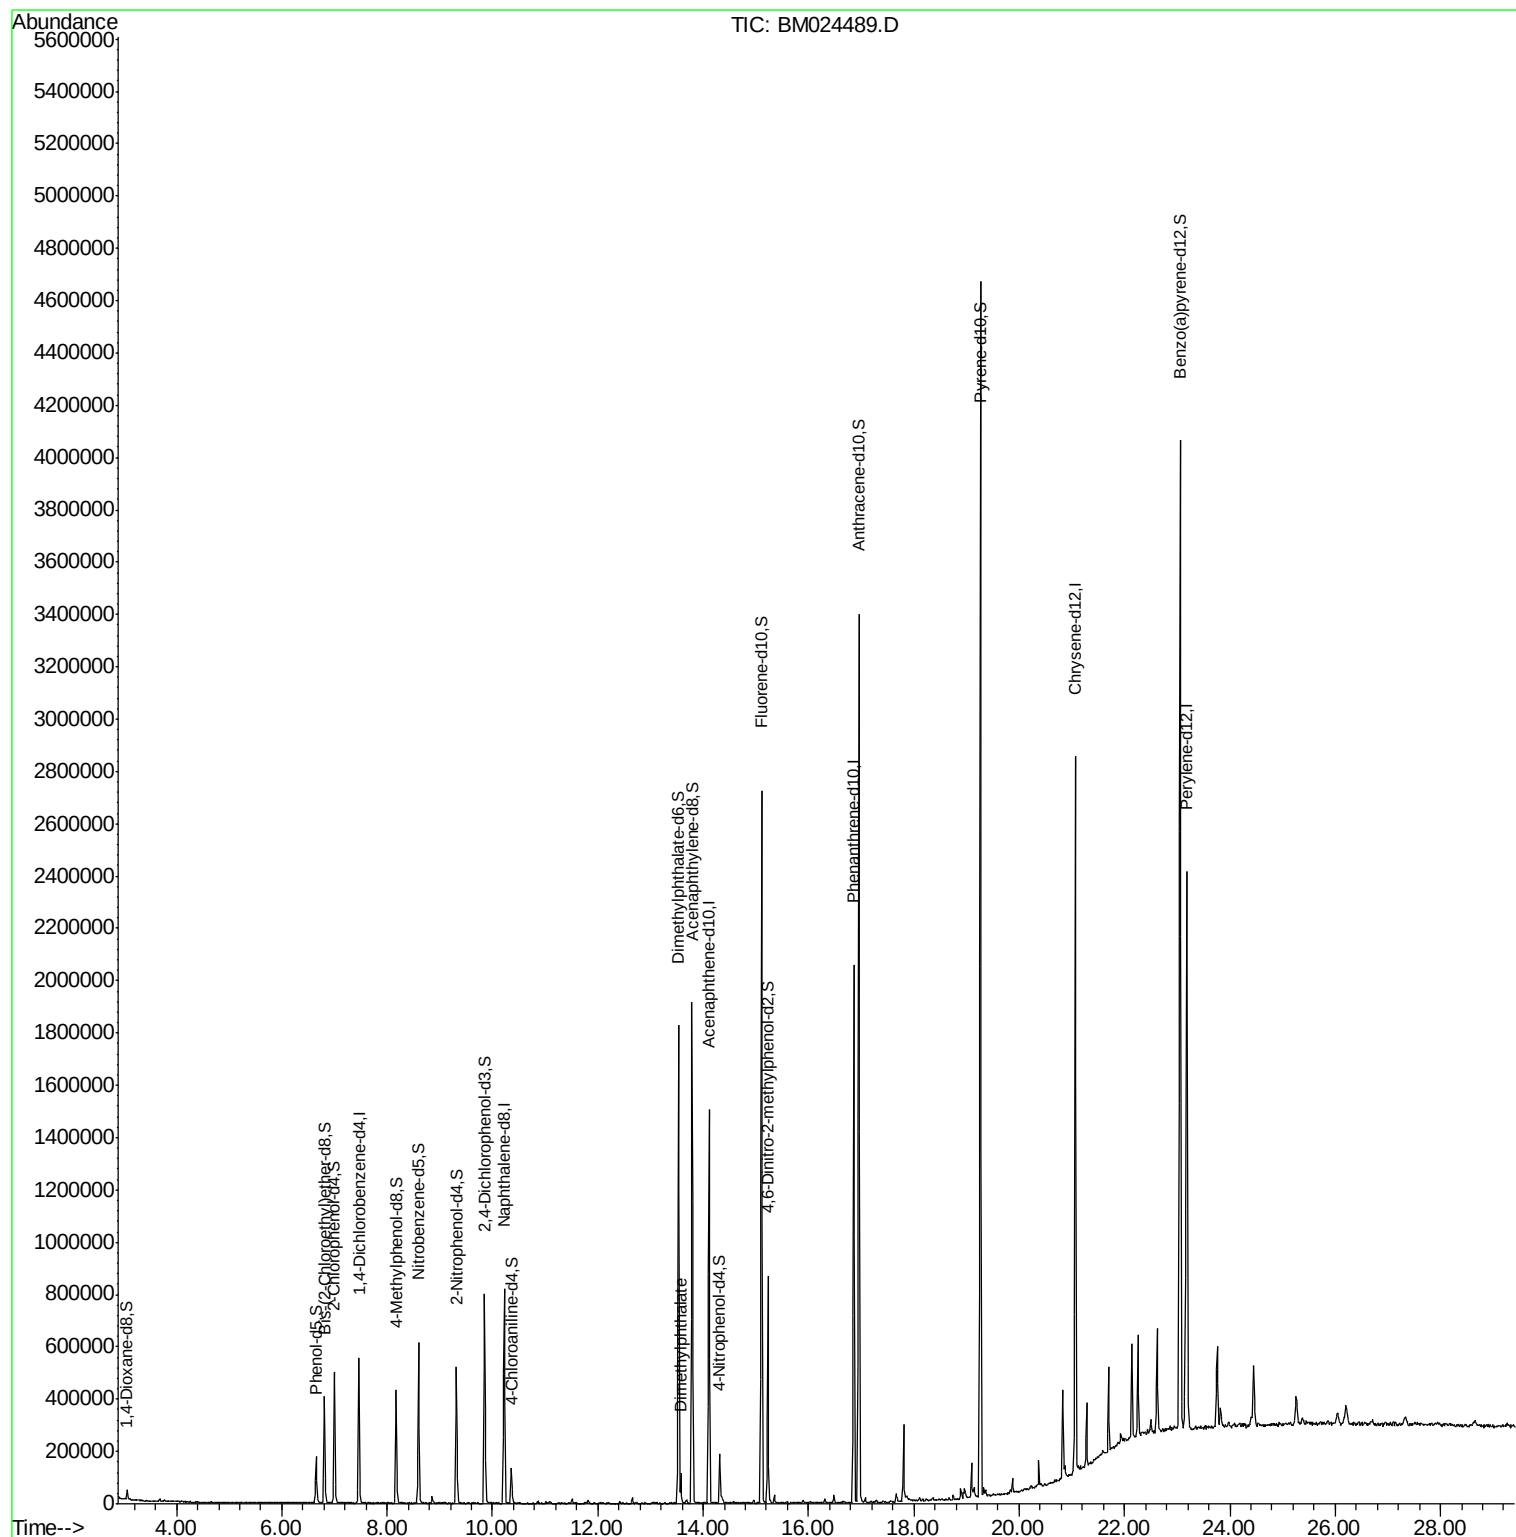

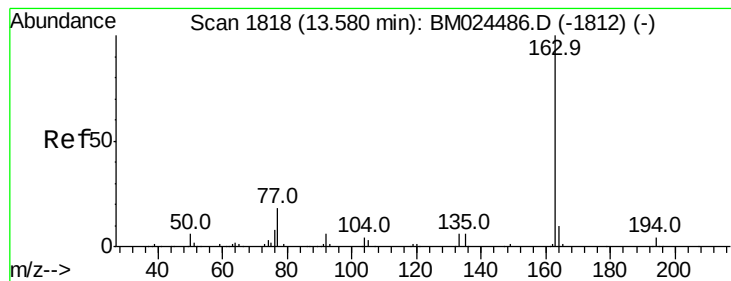

#45

Dimethylphthalate

Concen: 1.732 ng/ul

RT: 13.57 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM024489.D

Acq: 16 Jan 2020 11:26

Instrument :

BNA_M

ClientSampleId :

GASJ0


Tot Ion:163 Resp: 69550

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 9.6 8.0 12.0

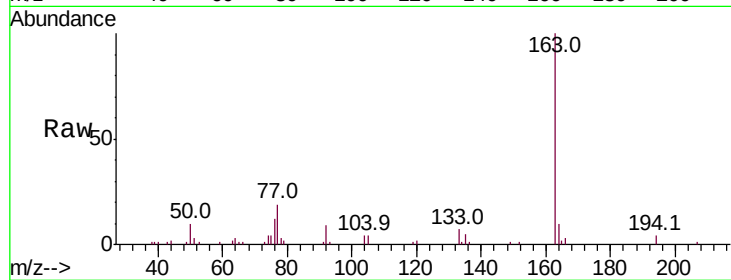

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

