

Data File : BM018608.D

Acq On : 17 Jan 2019 11:31

Operator : JU/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Jan 18 06:55:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jan 10 05:57:41 2019

Response via : Initial Calibration

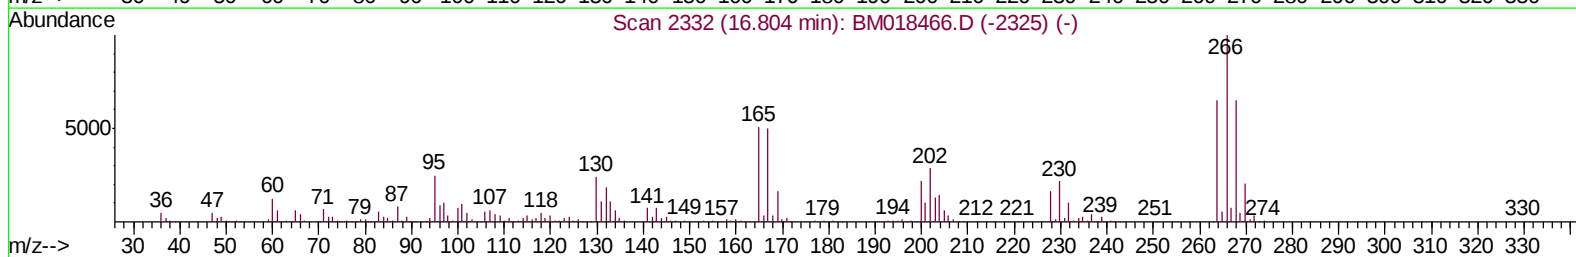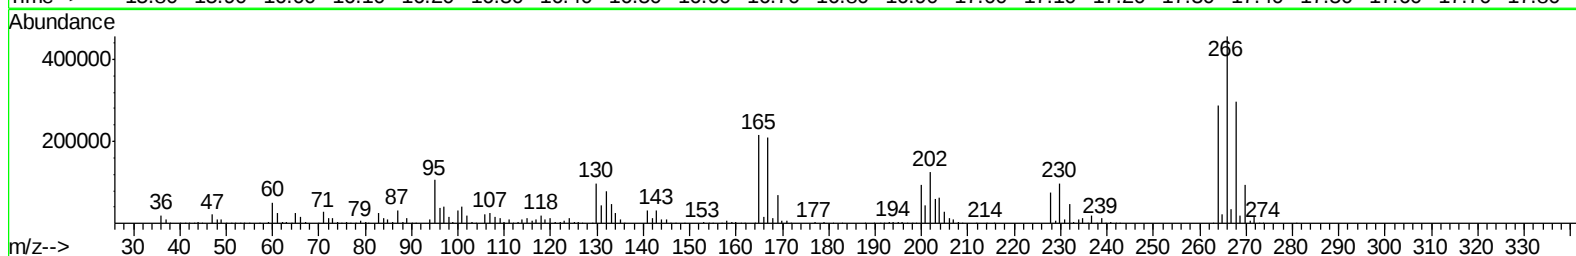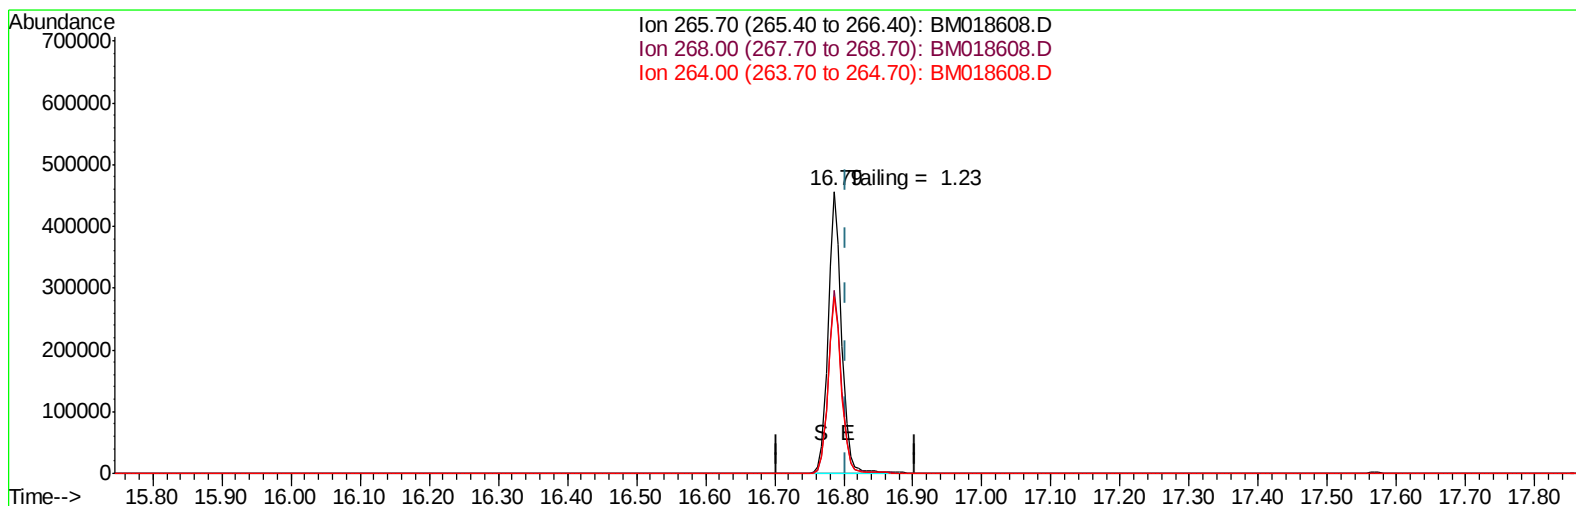

TIC: BM018608.D

(70) Pentachlorophenol (C)




16.786min (-0.017) 36952.75ng

response 612737

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.95
264.00	62.60	62.83
0.00	0.00	0.00

Data File : BM018608.D
Acq On : 17 Jan 2019 11:31
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 06:55:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

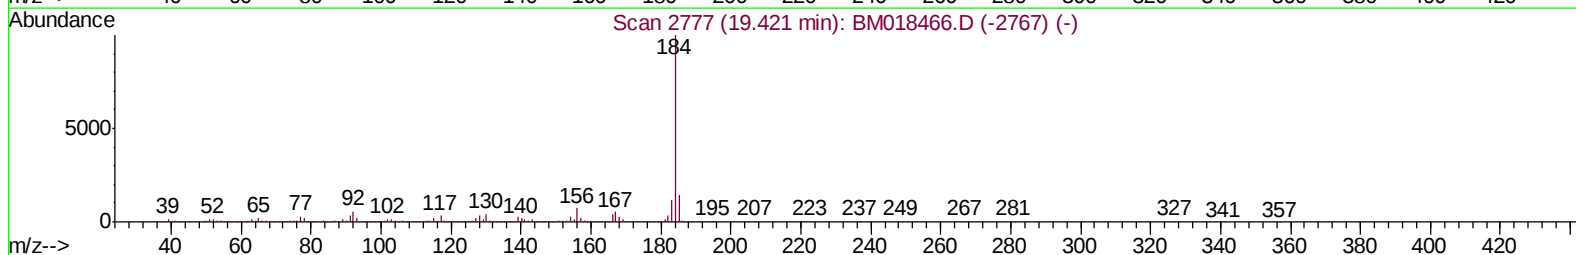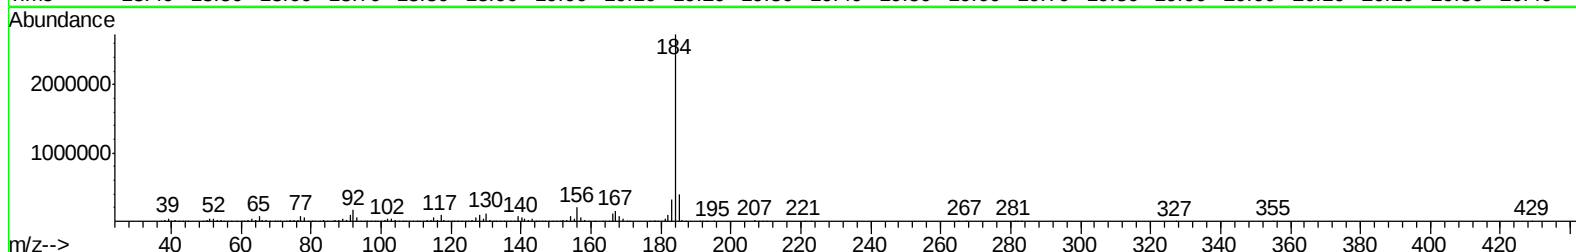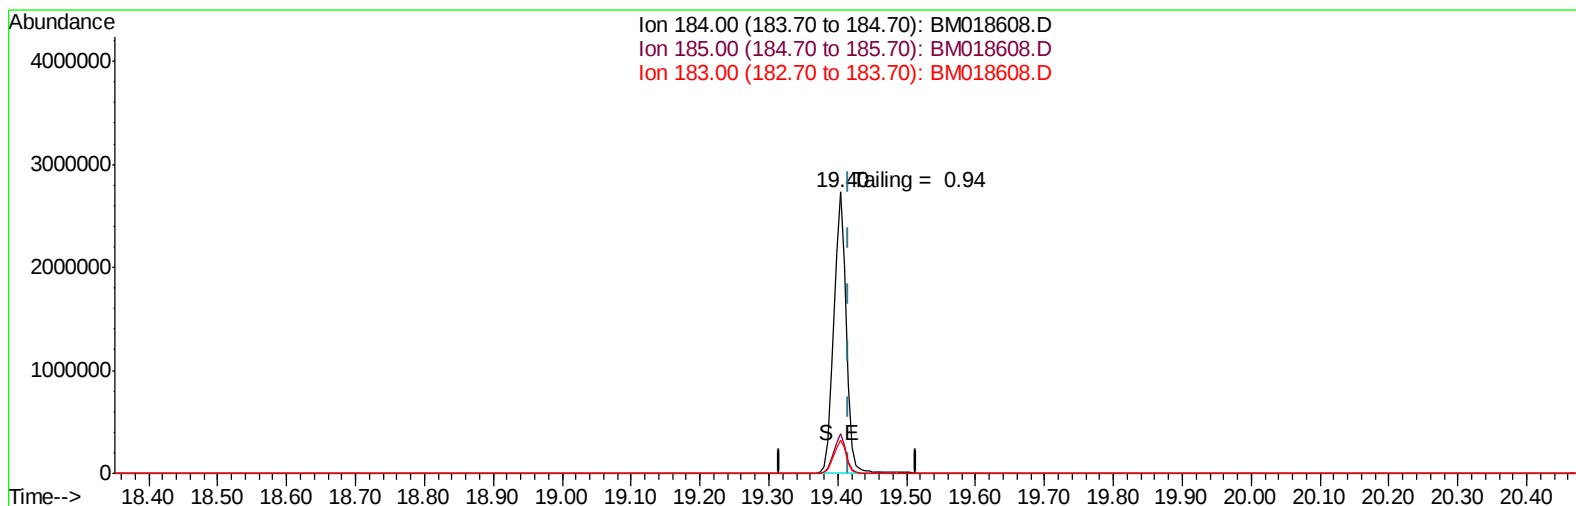

TIC: BM018608.D

(77) Benzidine

19.404min (-0.012) 28294.31ng

response 3414194

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.11
183.00	11.90	11.95
0.00	0.00	0.00