
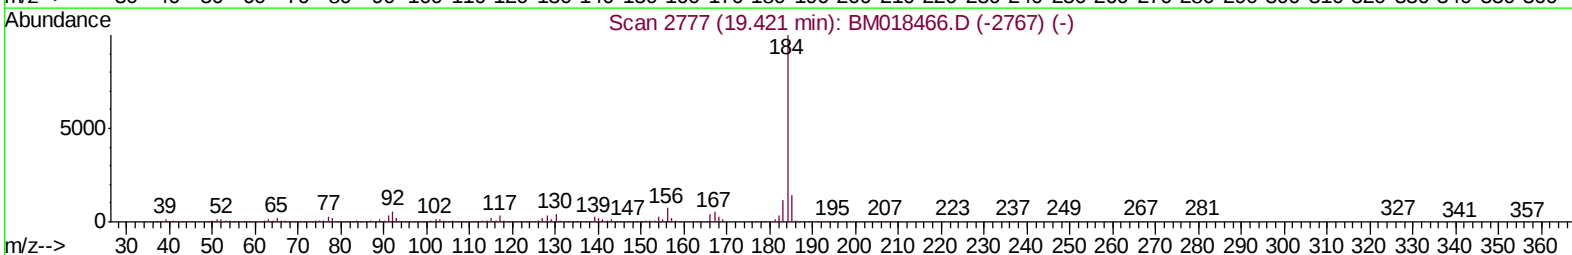
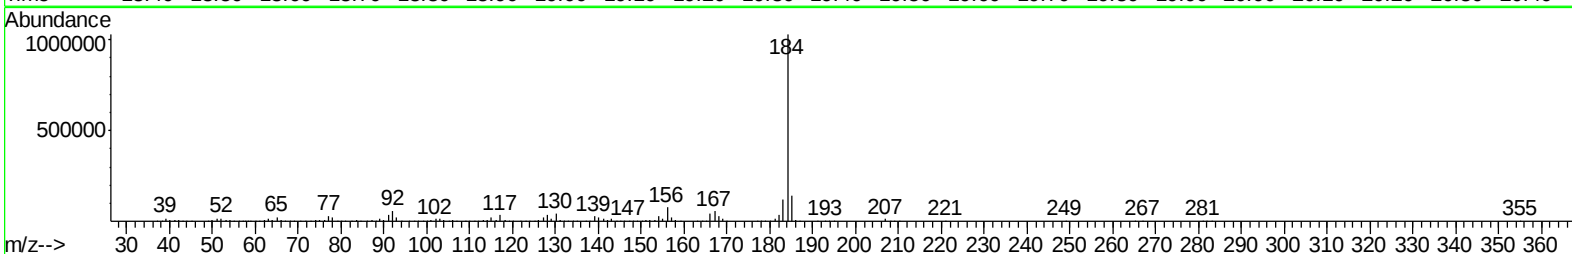


Data File : BM018628.D
Acq On : 18 Jan 2019 00:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 06:58:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

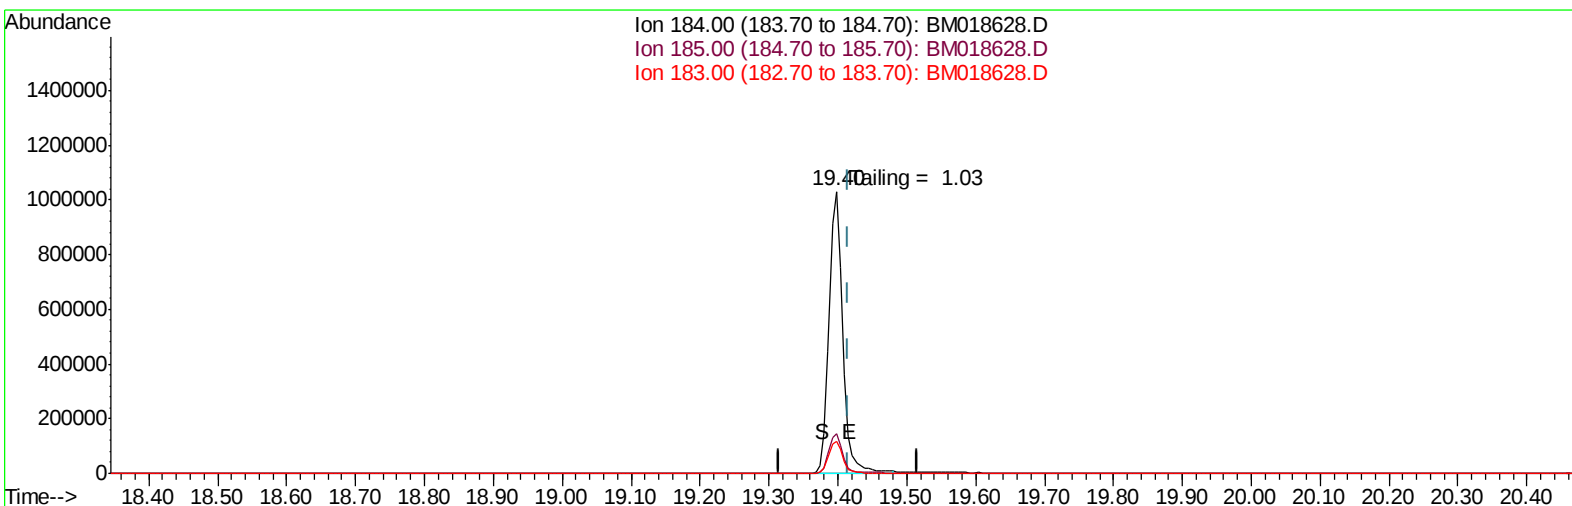

TIC: BM018628.D

(77) Benzidine




19.398min (-0.018) 4466.18ng

response 1419589

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.01
183.00	11.90	11.56
0.00	0.00	0.00

Data File : BM018628.D
Acq On : 18 Jan 2019 00:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 06:58:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

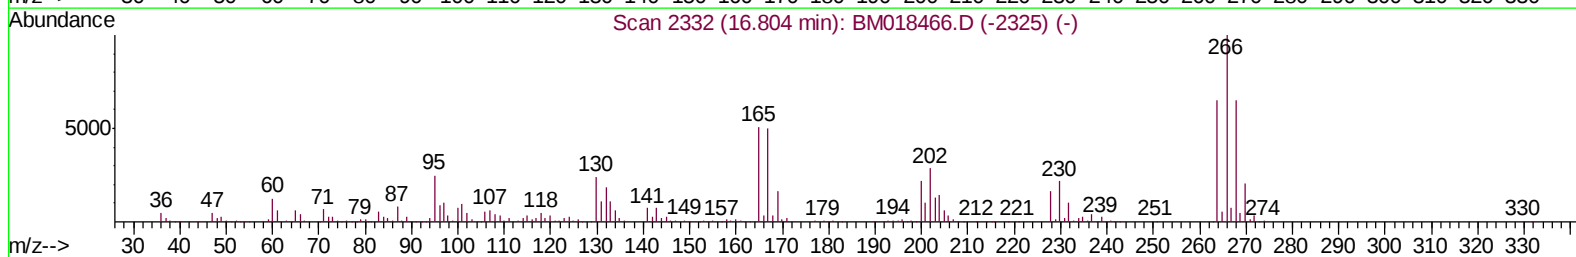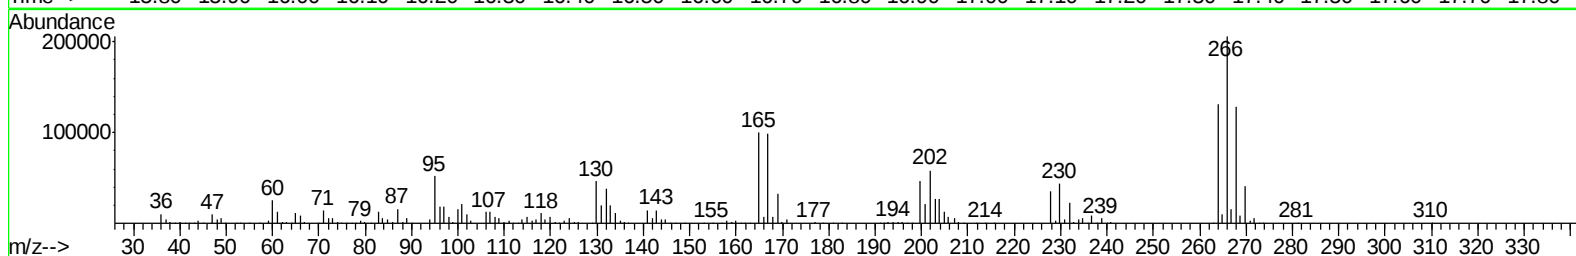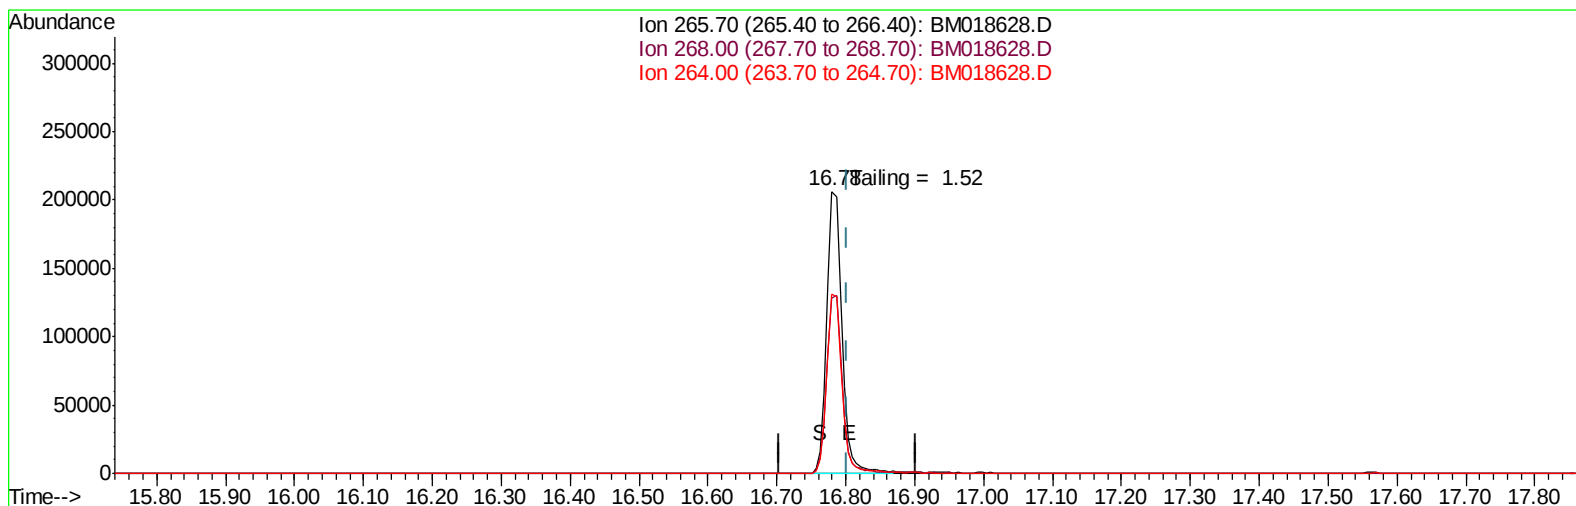

TIC: BM018628.D

(70) Pentachlorophenol (C)

16.780min (-0.023) 82579.15ng

response 313021

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.35
264.00	62.60	63.80
0.00	0.00	0.00