


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011719\
 Data File : BM018608.D
 Acq On : 17 Jan 2019 11:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

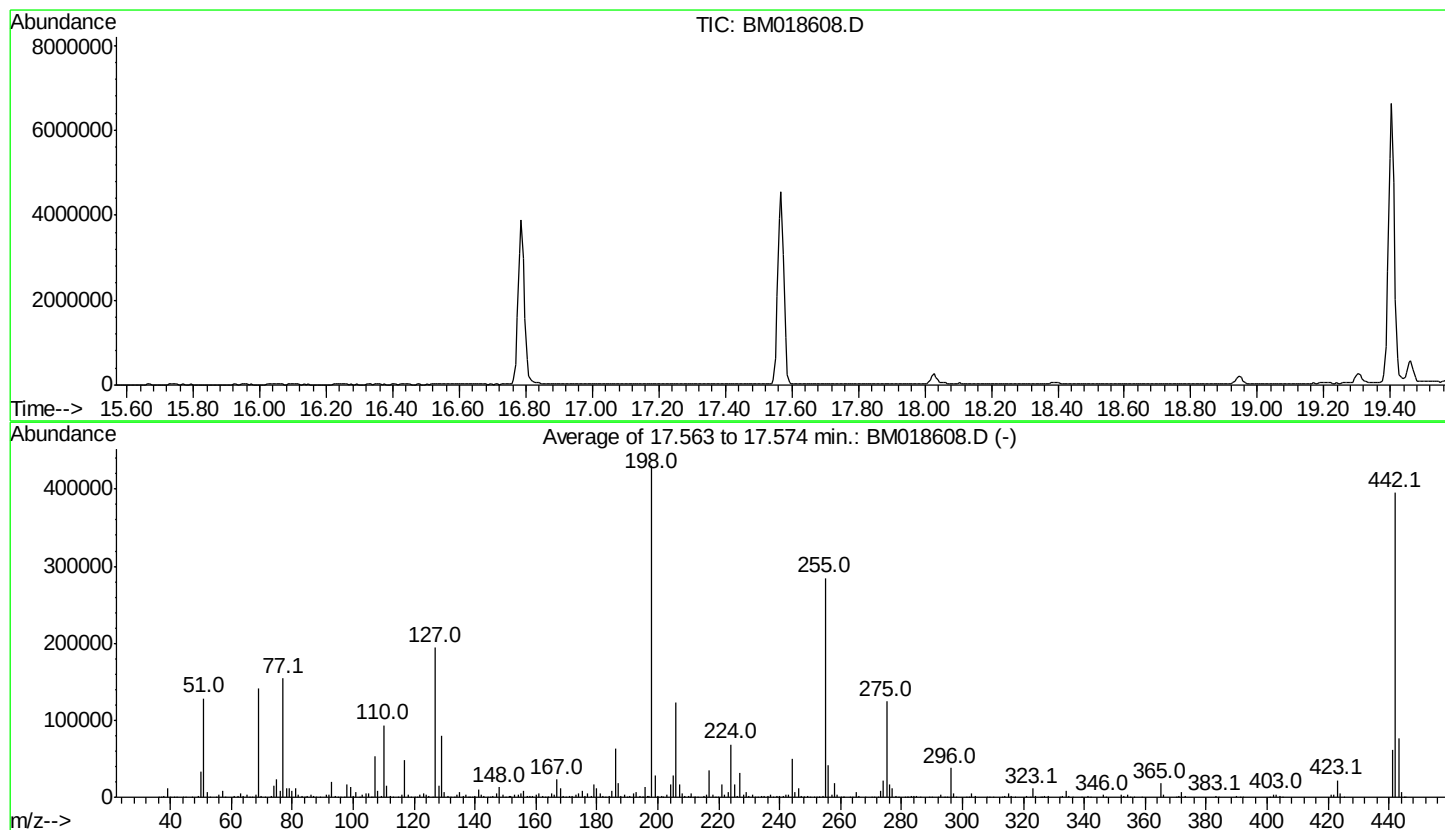

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	128301	PASS
68	69	0.00	2	2.0	2815	PASS
69	198	0.00	100	32.9	141789	PASS
70	69	0.00	2	0.7	926	PASS
127	198	10	80	45.0	193706	PASS
197	198	0.00	2	0.4	1718	PASS
198	198	100	100	100.0	430570	PASS
199	198	5	9	6.7	28840	PASS
275	198	10	60	28.9	124221	PASS
365	198	1	100	4.2	18142	PASS
441	198	0.01	100	14.2	61189	PASS
442	198	50	100	91.8	395306	PASS
443	442	15	24	19.2	75970	PASS