


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011719\
 Data File : BM018628.D
 Acq On : 18 Jan 2019 00:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

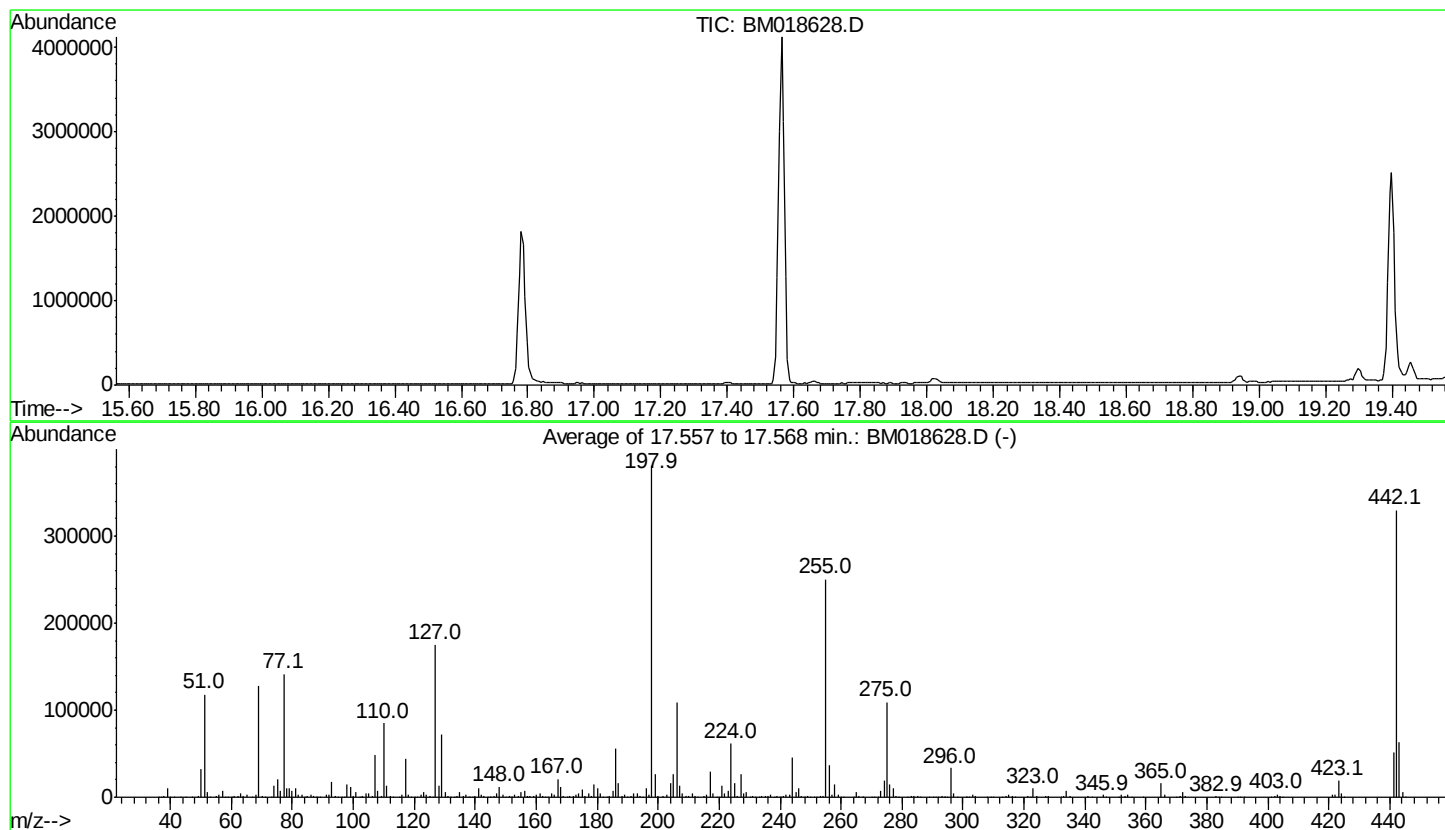

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	118328	PASS
68	69	0.00	2	2.0	2532	PASS
69	198	0.00	100	33.7	128502	PASS
70	69	0.00	2	0.6	813	PASS
127	198	10	80	46.1	175466	PASS
197	198	0.00	2	0.6	2281	PASS
198	198	100	100	100.0	380864	PASS
199	198	5	9	6.9	26354	PASS
275	198	10	60	28.7	109456	PASS
365	198	1	100	4.2	15840	PASS
441	198	0.01	100	13.6	51784	PASS
442	198	50	100	86.6	329856	PASS
443	442	15	24	19.2	63213	PASS