
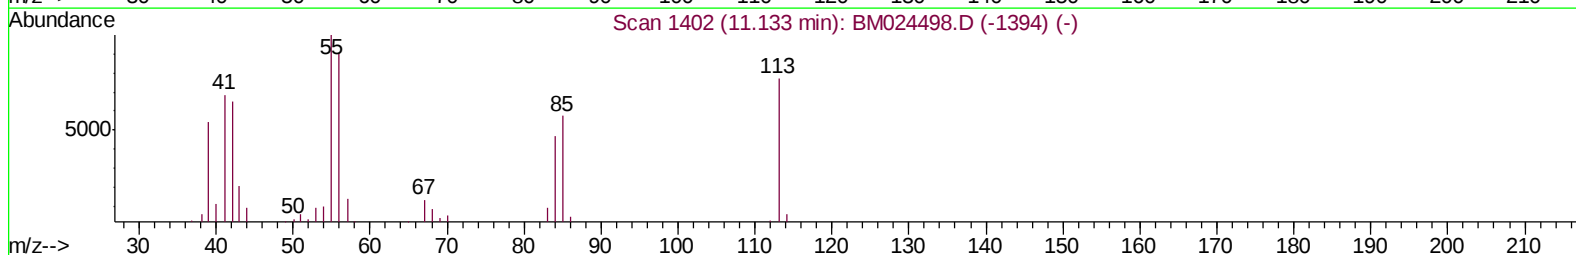
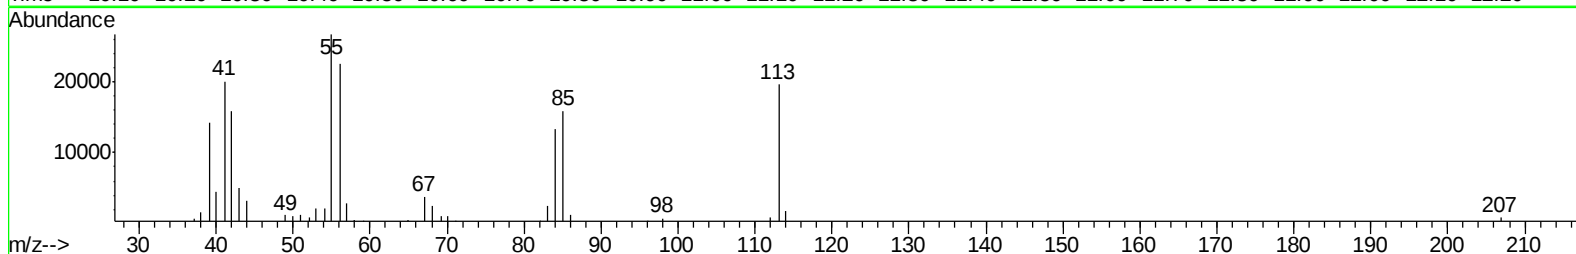


Data File : BM024515.D
Acq On : 18 Jan 2020 02:55
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jan 18 04:51:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 18 00:06:51 2020
Response via : Initial Calibration

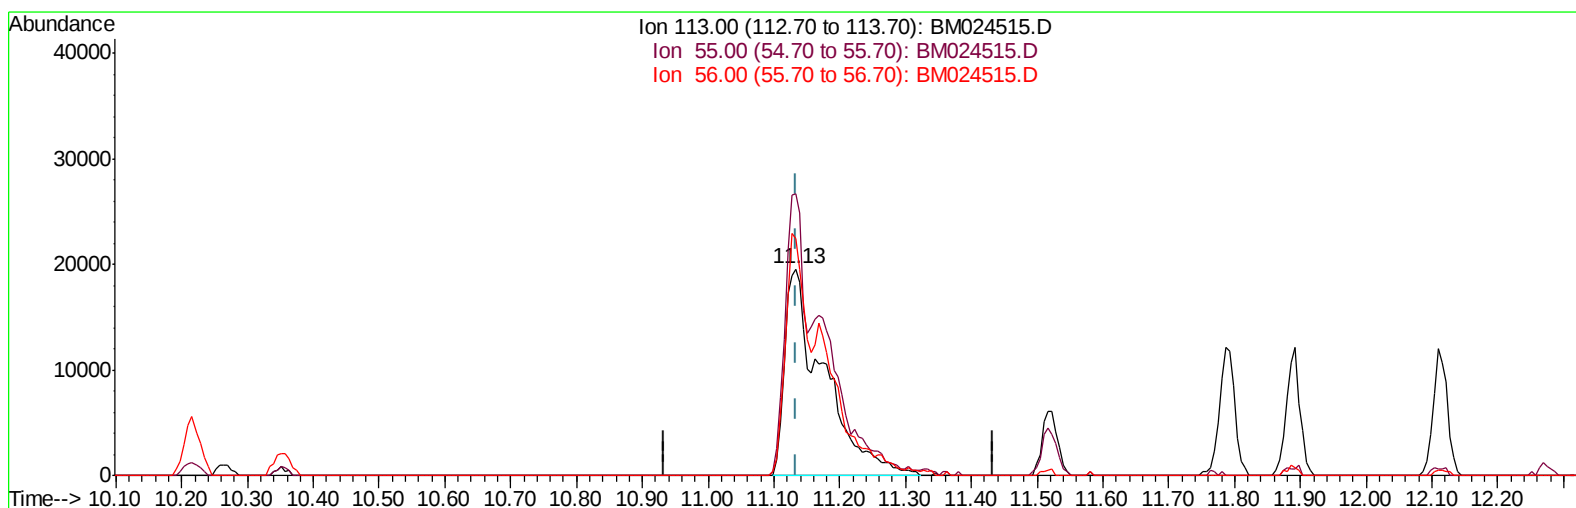

TIC: BM024515.D

(32) Caprolactam

11.134min (+0.000) 20.23ng/ul m

response 80116

Ion	Exp%	Act%
113.00	100	100
55.00	147.90	136.30
56.00	113.50	114.80
0.00	0.00	0.00