
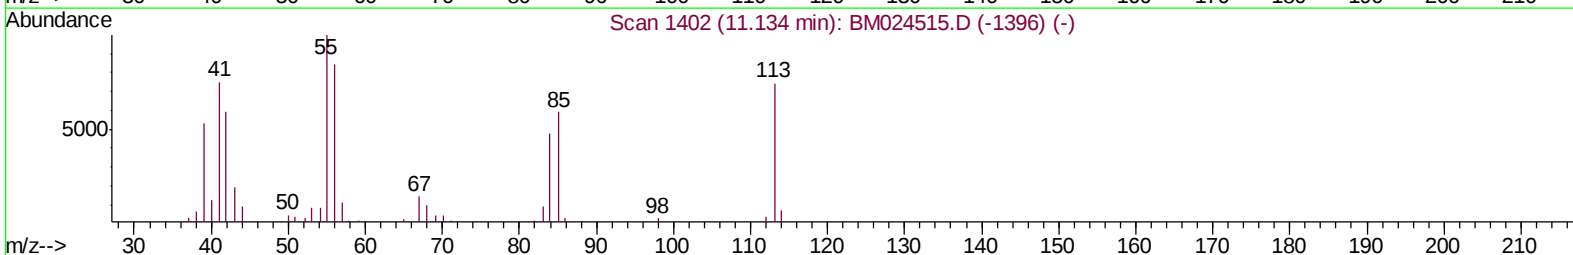
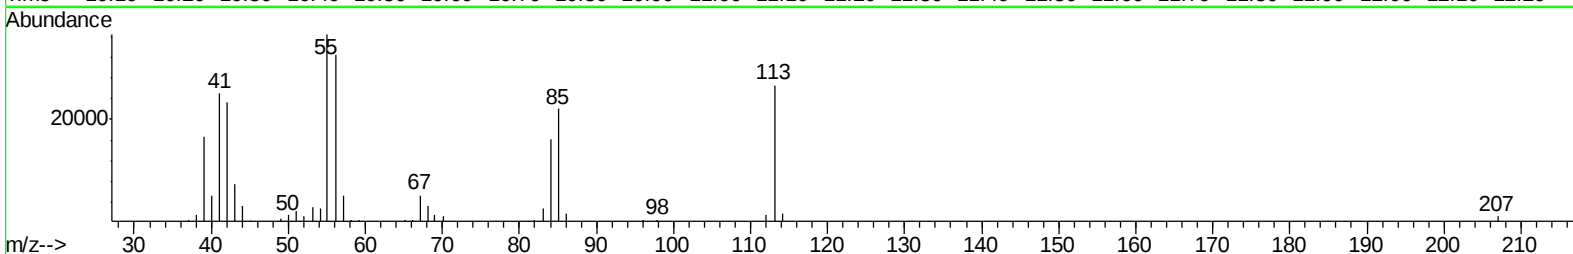


Data File : BM024532.D
Acq On : 18 Jan 2020 13:01
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Jan 20 03:23:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 01:02:24 2020
Response via : Initial Calibration

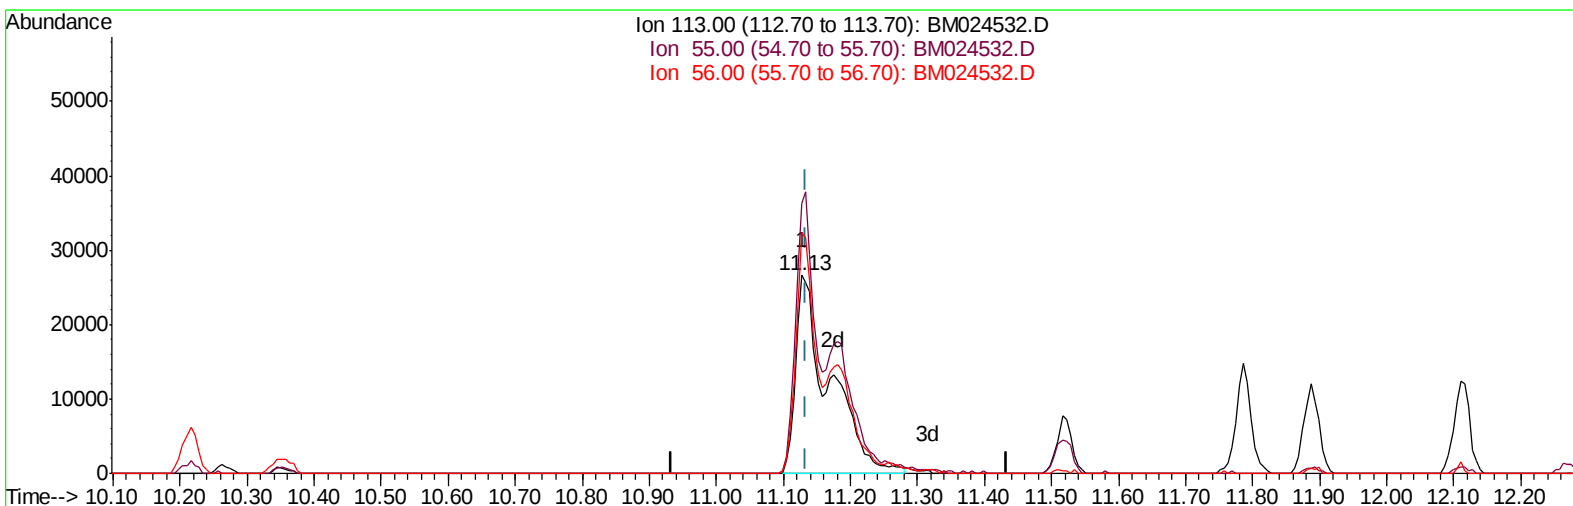

TIC: BM024532.D

(32) Caprolactam

11.128min (-0.006) 20.72ng/ul m

response 93353

Ion	Exp%	Act%
113.00	100	100
55.00	147.90	136.85
56.00	113.50	121.81
0.00	0.00	0.00