
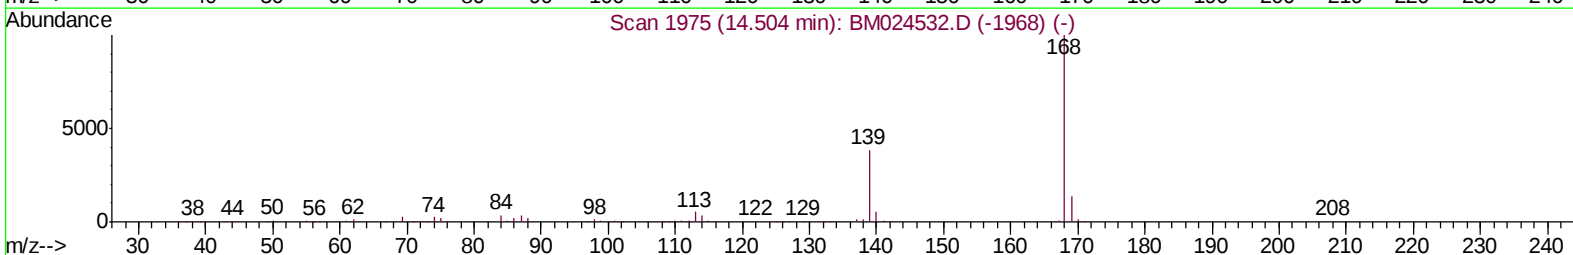
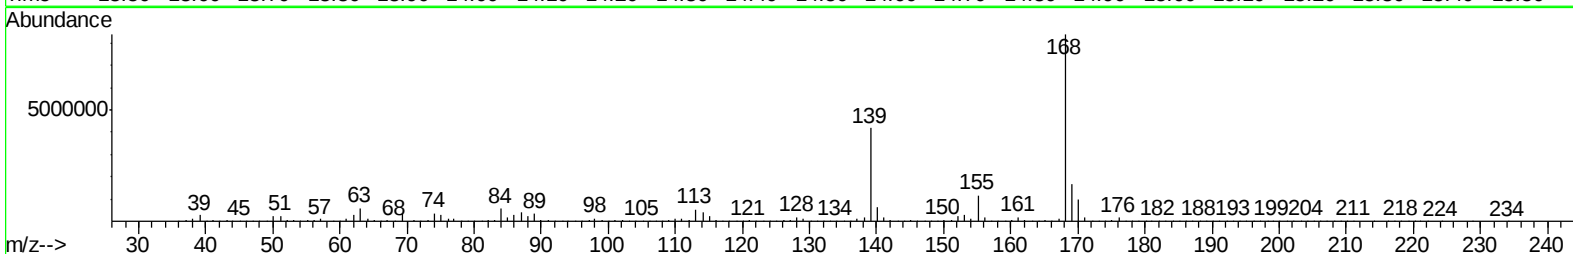


Data File : BM024537.D
Acq On : 18 Jan 2020 16:00
Operator : JU
Sample : L1109-11
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Jan 20 03:28:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

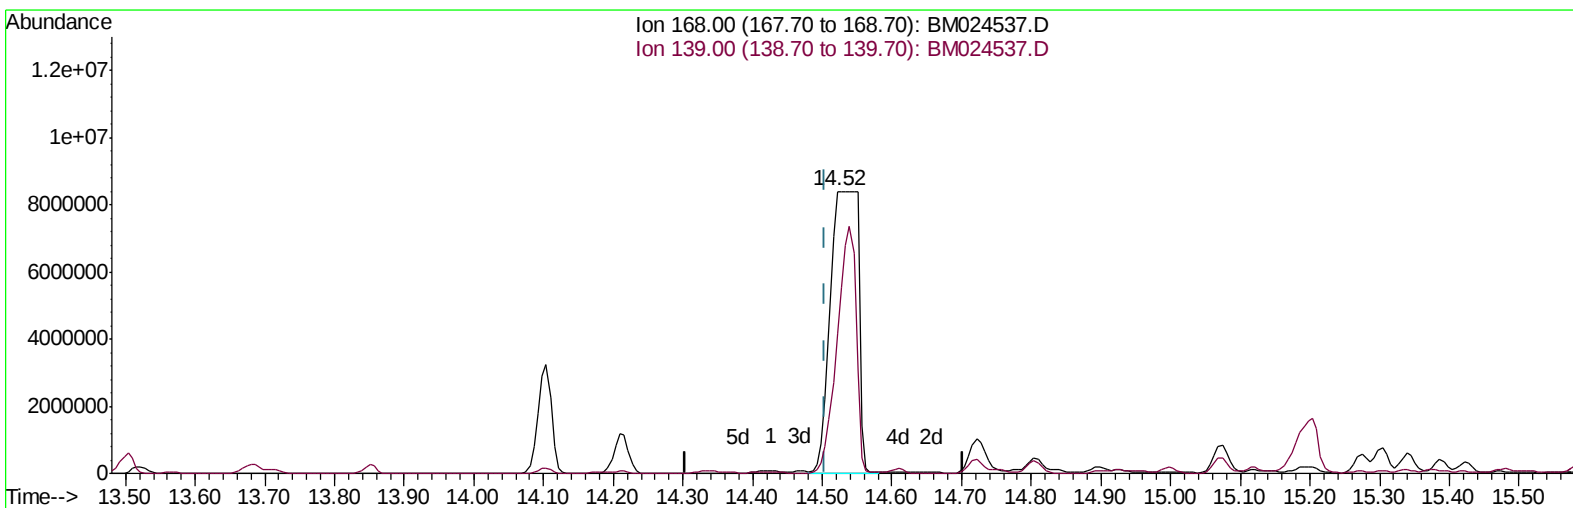

TIC: BM024537.D

(54) Dibenzofuran

14.521min (+0.018) 407.26ng/ul m

response 23553244

Ion	Exp%	Act%
168.00	100	100
139.00	38.40	49.73#
0.00	0.00	0.00
0.00	0.00	0.00