
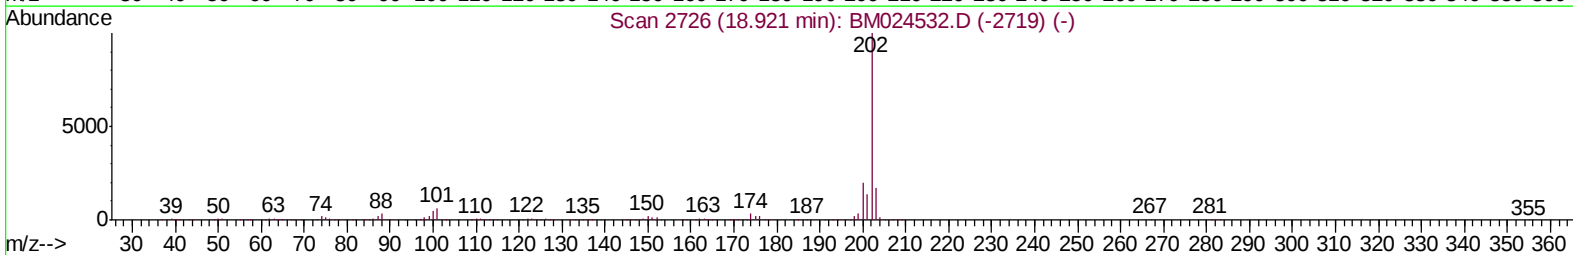
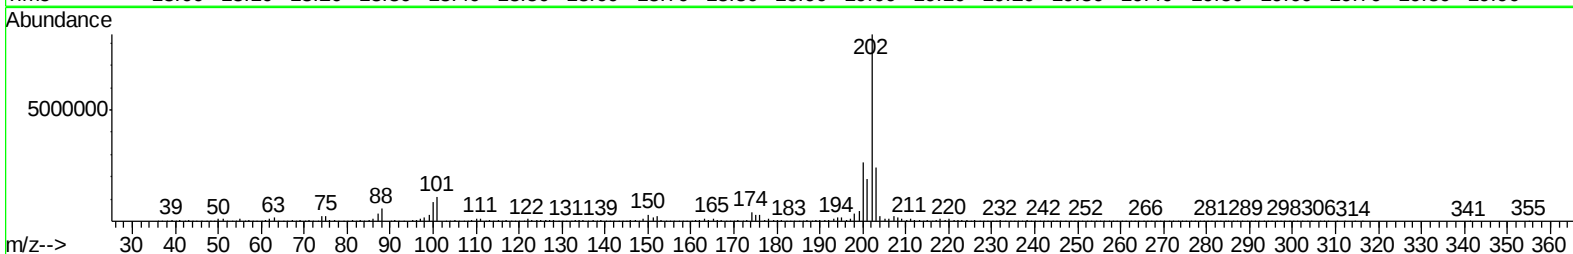


Data File : BM024537.D
Acq On : 18 Jan 2020 16:00
Operator : JU
Sample : L1109-11
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Jan 20 04:21:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

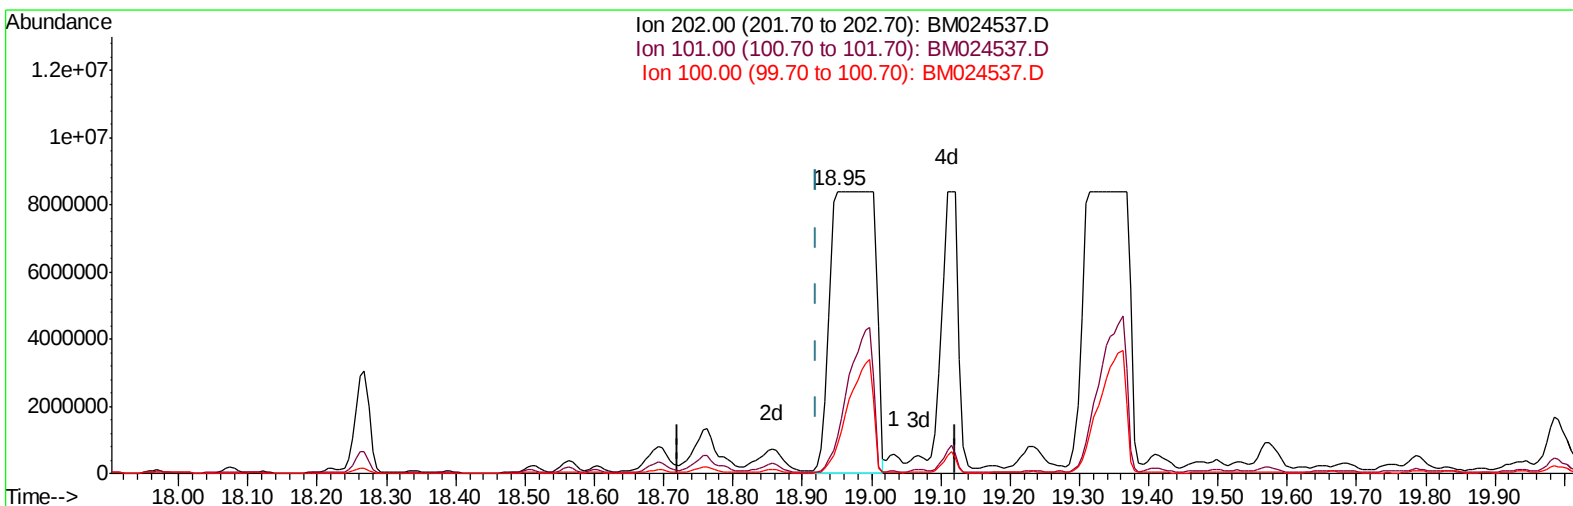

TIC: BM024537.D

(77) Fluoranthene (C)

18.951min (+0.029) 412.92ng/ul m

response 36935465

Ion	Exp%	Act%
202.00	100	100
101.00	6.80	13.34#
100.00	5.40	10.38#
0.00	0.00	0.00