
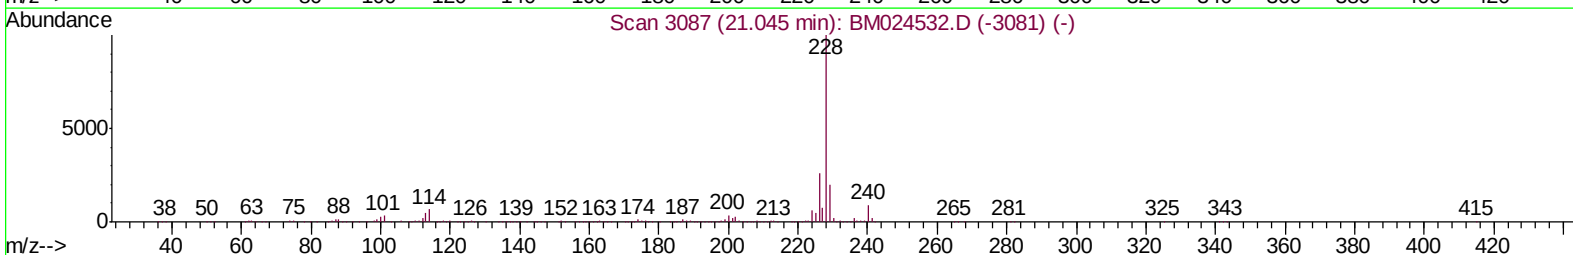
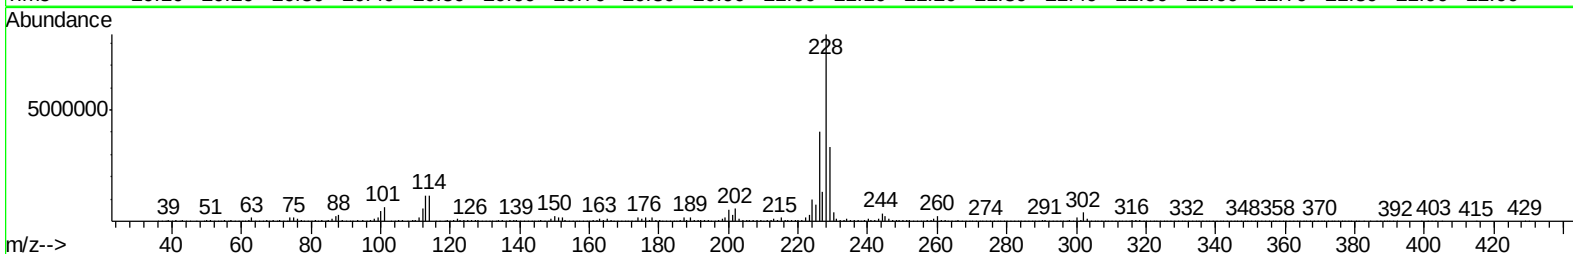


Data File : BM024538.D
Acq On : 18 Jan 2020 16:35
Operator : JU
Sample : L1109-10 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Jan 20 03:29:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

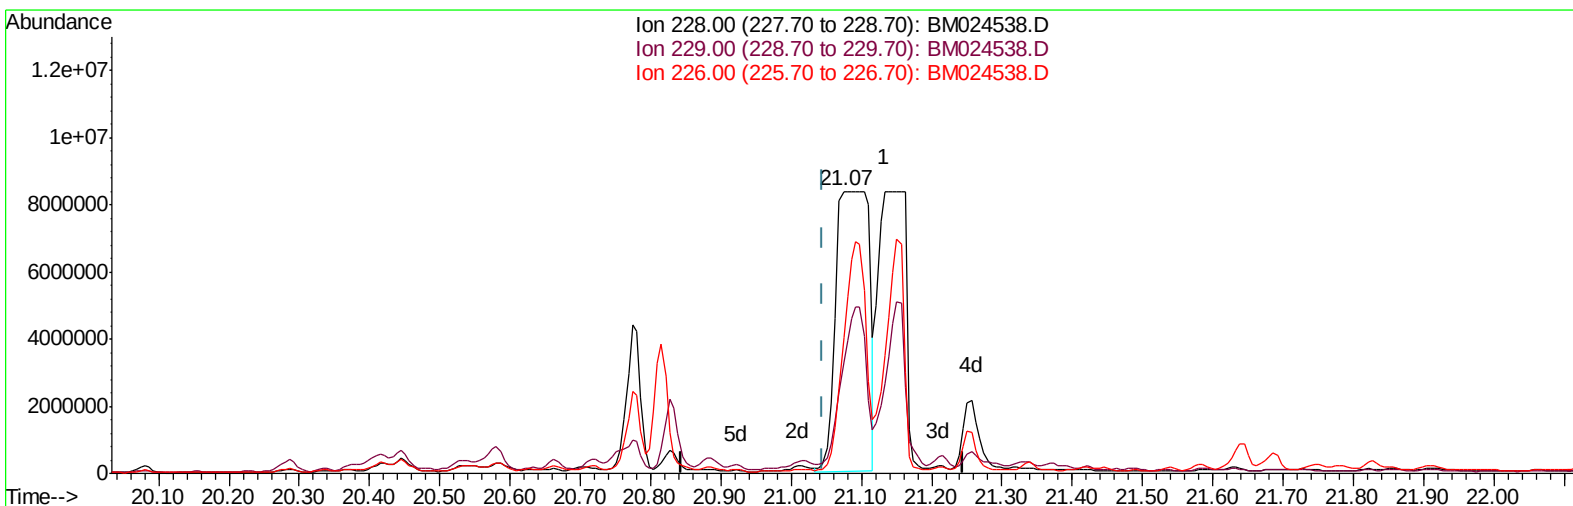

TIC: BM024538.D

(83) Benzo(a)anthracene
21.074min (+0.030) 214.11ng/ul m
response 27417434

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	39.72#
226.00	26.40	48.14#
0.00	0.00	0.00