
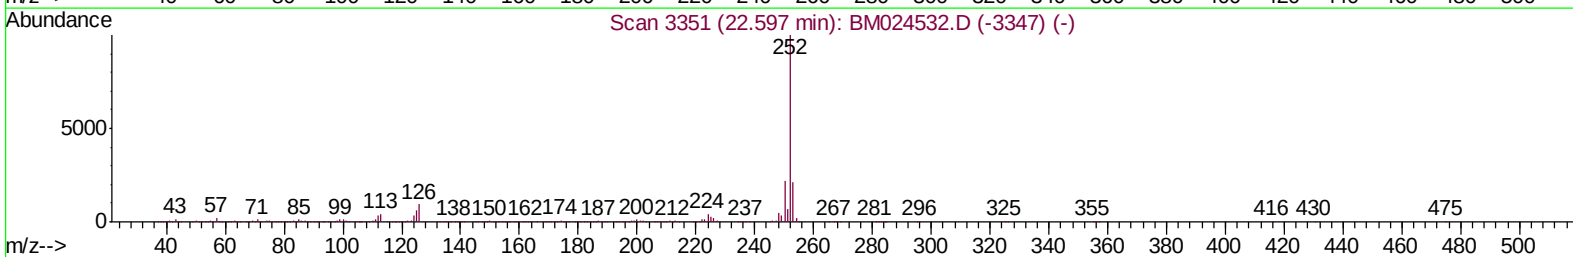
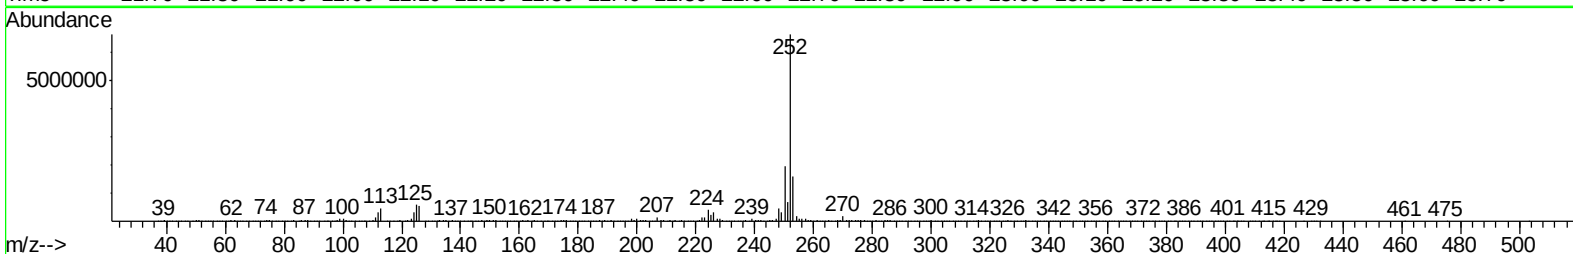


Data File : BM024539.D
Acq On : 18 Jan 2020 17:11
Operator : JU
Sample : L1109-09 5X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jan 20 05:01:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

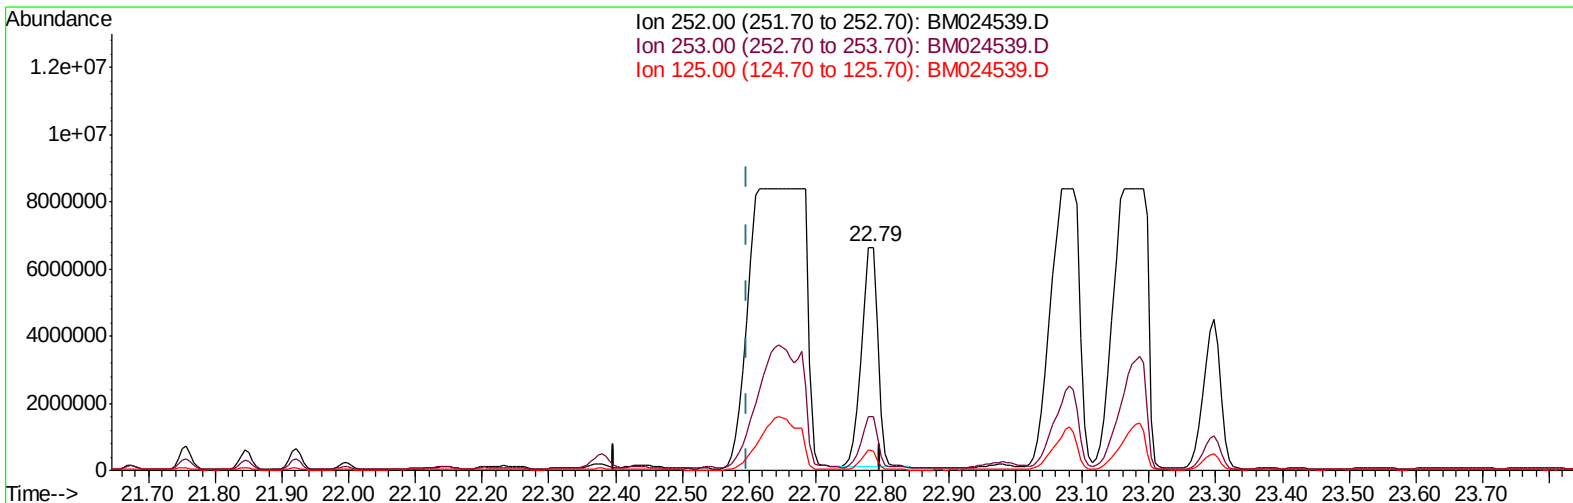

TIC: BM024539.D

(89) Benzo(k)fluoranthene

22.786min (+0.188) 99.96ng/ul

response 10725420

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.95
125.00	6.50	8.64#
0.00	0.00	0.00