
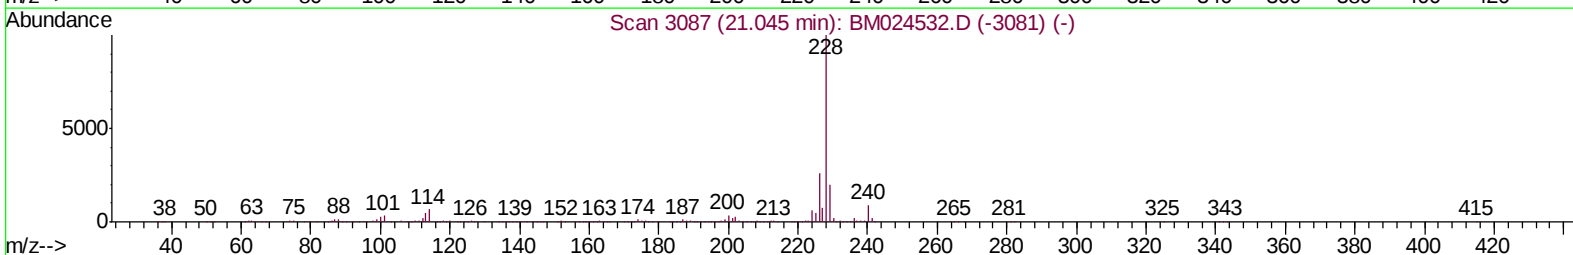
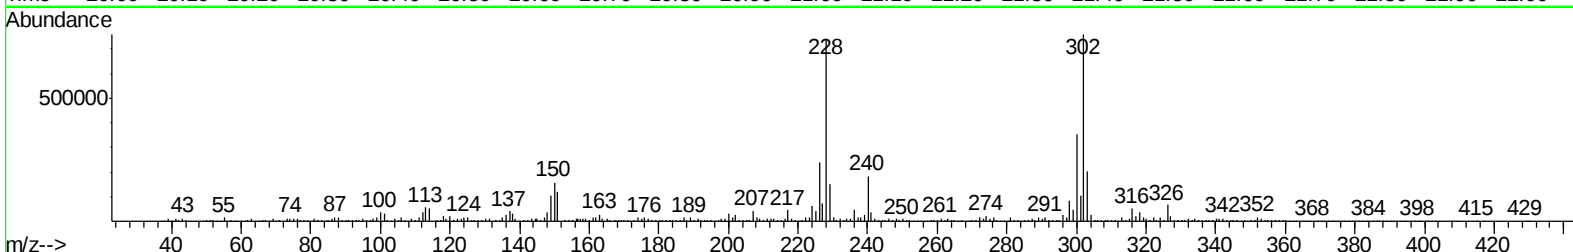


Data File : BM024540.D
Acq On : 18 Jan 2020 17:47
Operator : JU
Sample : L1109-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Quant Time: Jan 20 03:30:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

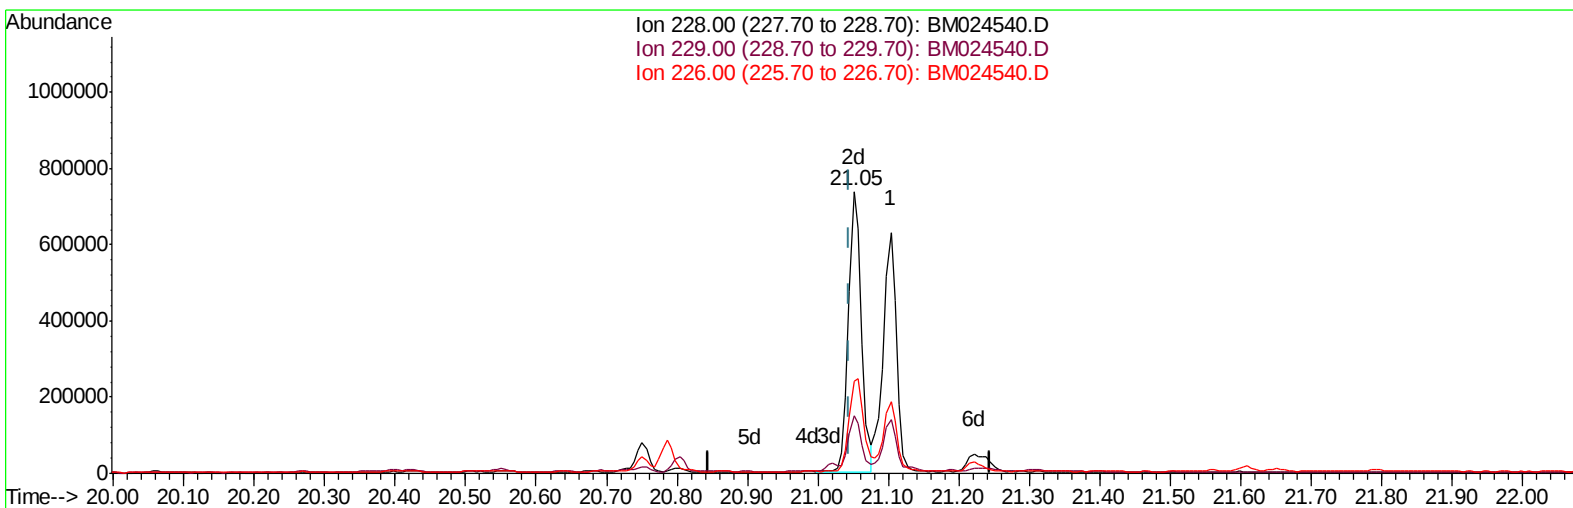

TIC: BM024540.D

(83) Benzo(a)anthracene

21.051min (+0.006) 7.75ng/ul m

response 930795

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	20.65
226.00	26.40	32.62#
0.00	0.00	0.00