
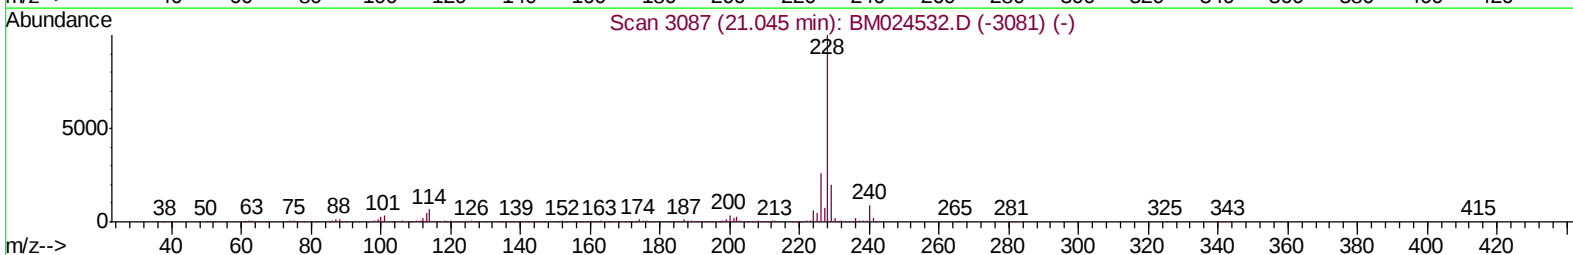
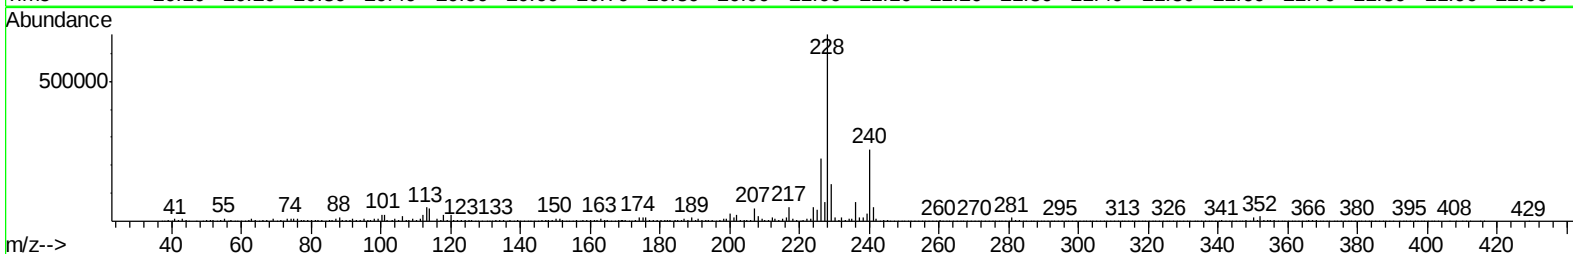


Data File : BM024542.D
Acq On : 18 Jan 2020 18:58
Operator : JU
Sample : L1109-03MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Jan 20 03:30:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

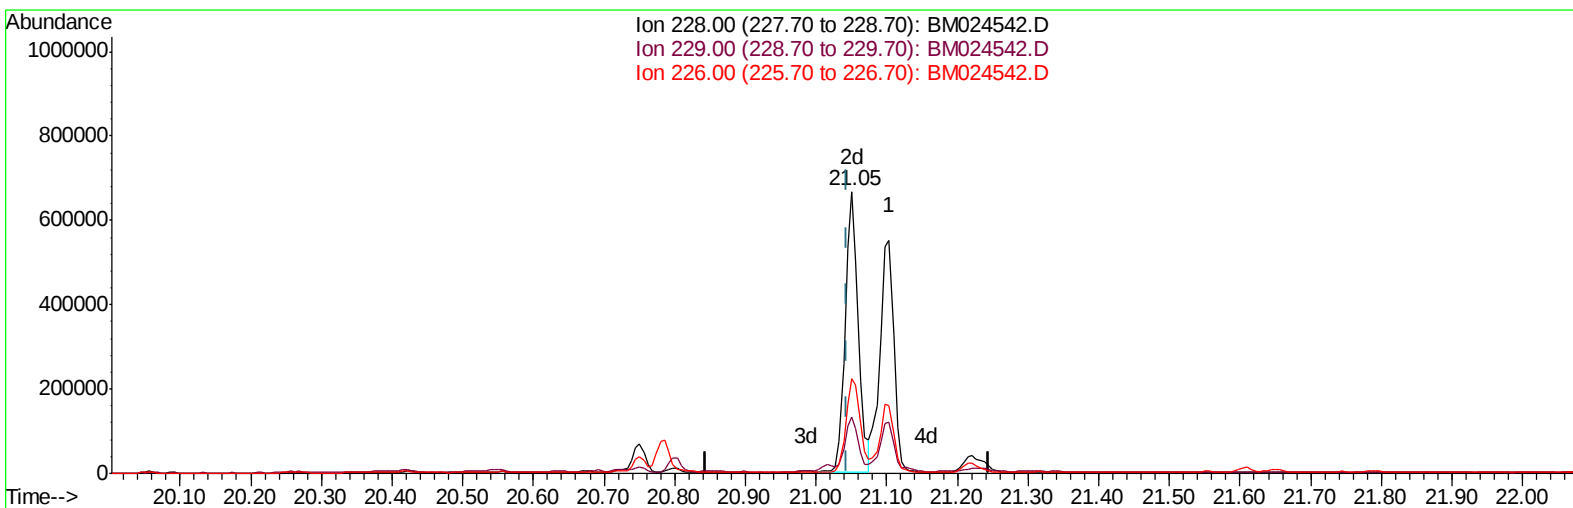

TIC: BM024542.D

(83) Benzo(a)anthracene

21.050min (+0.006) 8.04ng/ul m

response 854722

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	20.11
226.00	26.40	33.61#
0.00	0.00	0.00