
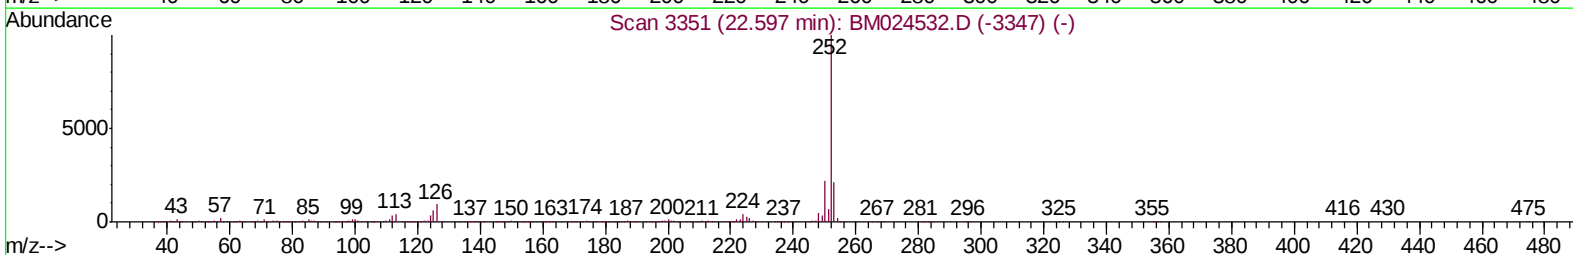
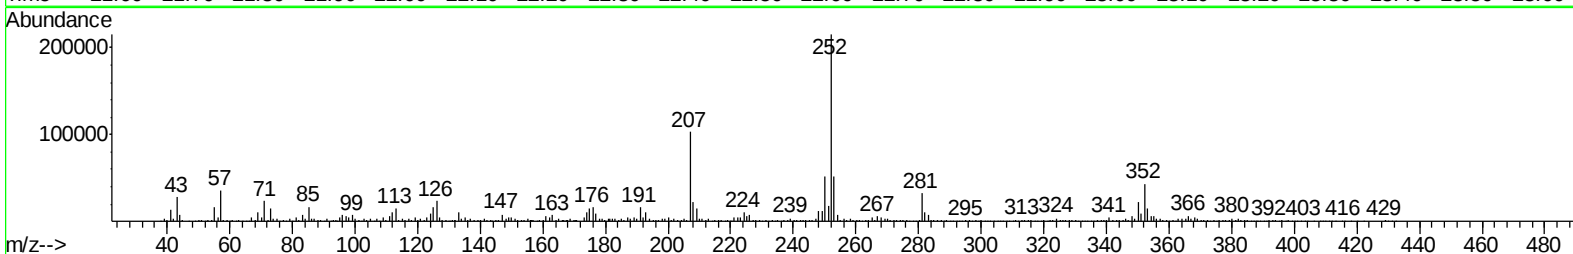


Data File : BM024542.D
Acq On : 18 Jan 2020 18:58
Operator : JU
Sample : L1109-03MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Jan 20 03:30:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

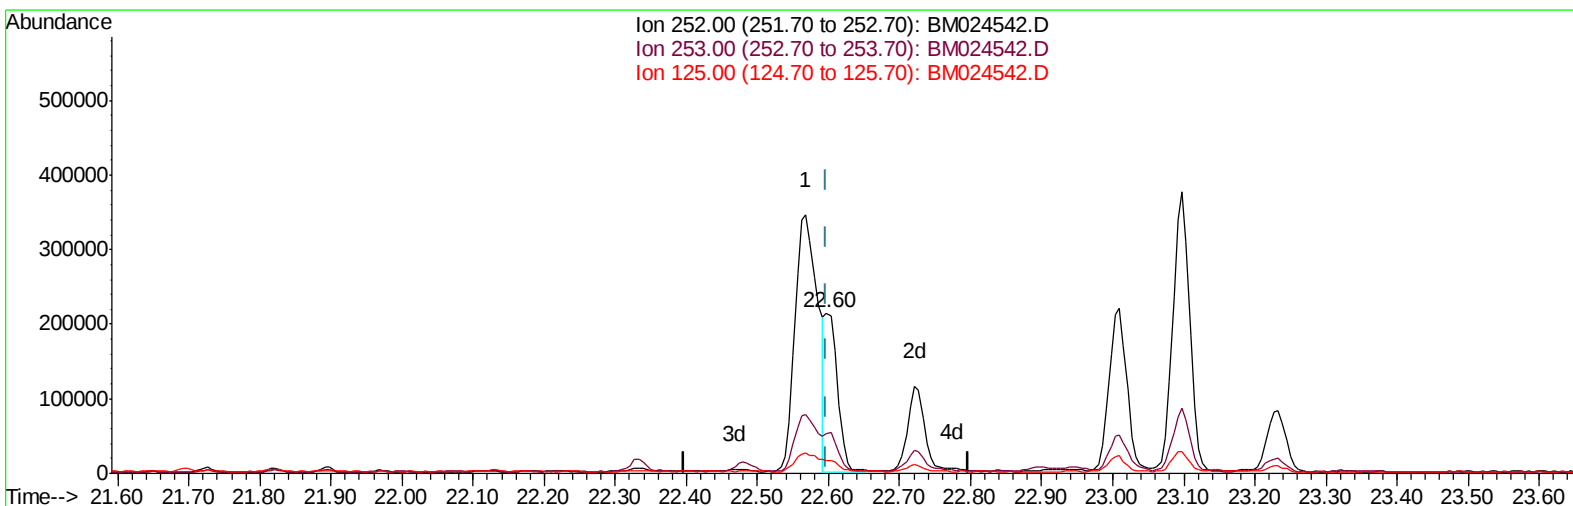

TIC: BM024542.D

(89) Benzo(k)fluoranthene

22.597min (-0.000) 2.29ng/ul m

response 259796

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	24.35
125.00	6.50	7.95#
0.00	0.00	0.00