
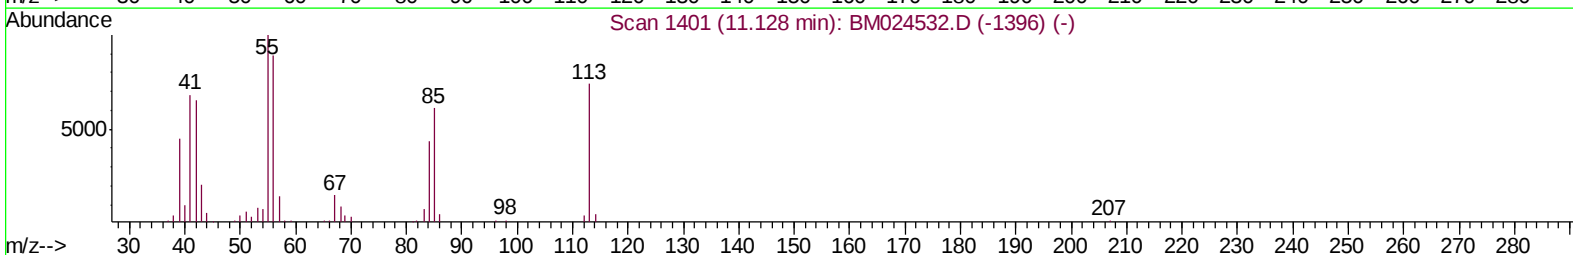
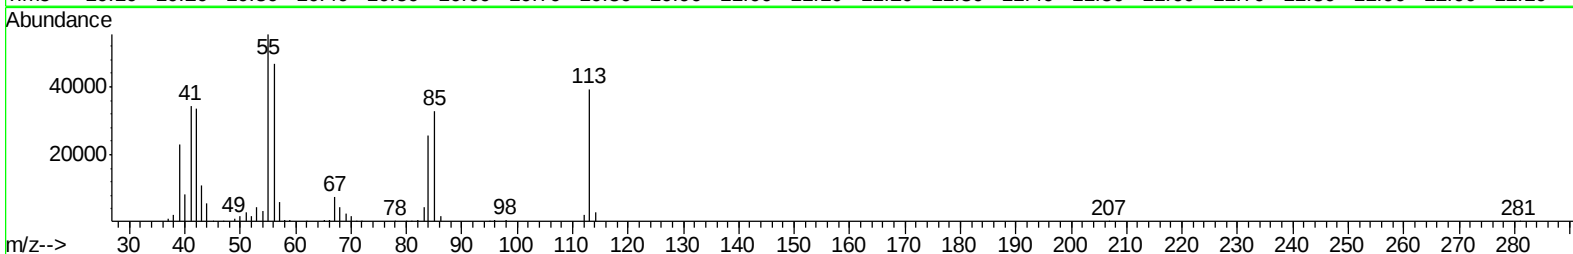


Data File : BM024543.D
Acq On : 18 Jan 2020 19:34
Operator : JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 47 Sample Multiplier: 1

Quant Time: Jan 20 03:30:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

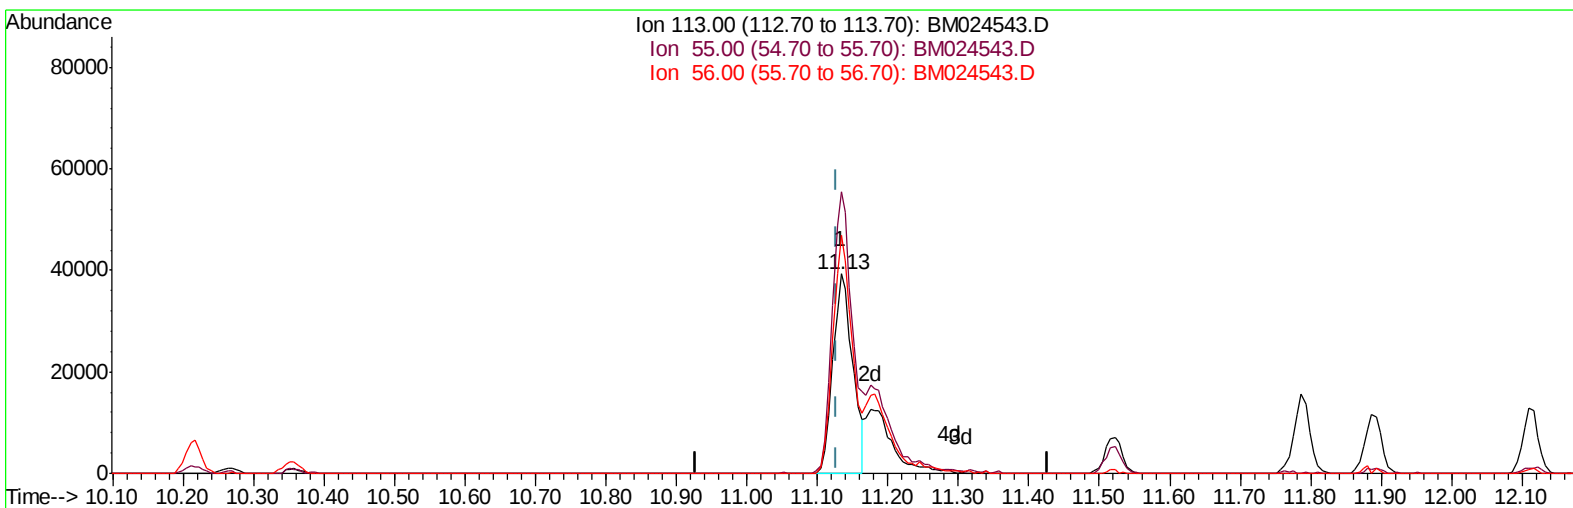

TIC: BM024543.D

(32) Caprolactam

11.134min (+0.006) 15.96ng/ul

response 76492

Ion	Exp%	Act%
113.00	100	100
55.00	147.90	141.11
56.00	113.50	119.20
0.00	0.00	0.00