

Data File : BM024524.D
Acq On : 18 Jan 2020 08:16
Operator : JU
Sample : PB126169BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK69

Quant Time: Jan 20 01:05:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 01:02:24 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	188744	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	839952	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	629976	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1483161	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1535669	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	1594966	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	29008	7.51	ng/uL	0.00
5) Phenol-d5	6.65	99	470751	33.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	281510	36.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	439308	36.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	434276	33.67	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	230660	39.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	273209	42.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	505713	35.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	690885	43.20	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1856115	37.60	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	2129798	37.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	288518	35.02	ng/ul	0.00
58) Fluorene-d10	15.10	176	1607720	37.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	274794	32.46	ng/ul	0.00
71) Anthracene-d10	16.95	188	2591434	37.57	ng/ul	0.00
79) Pyrene-d10	19.26	212	3019847	36.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	3045958	36.82	ng/ul	0.00


Target Compounds				Qvalue		
15) N-Nitroso-di-n-propylamine	8.17	70	10878	1.136 ng/ul#	1	
46) 2,6-Dinitrotoluene	13.53	165	14212	1.505 ng/ul#	39	


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM024524.D
Acq On : 18 Jan 2020 08:16
Operator : JU
Sample : PB126169BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK69

Quant Time: Jan 20 01:05:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 01:02:24 2020
Response via : Initial Calibration

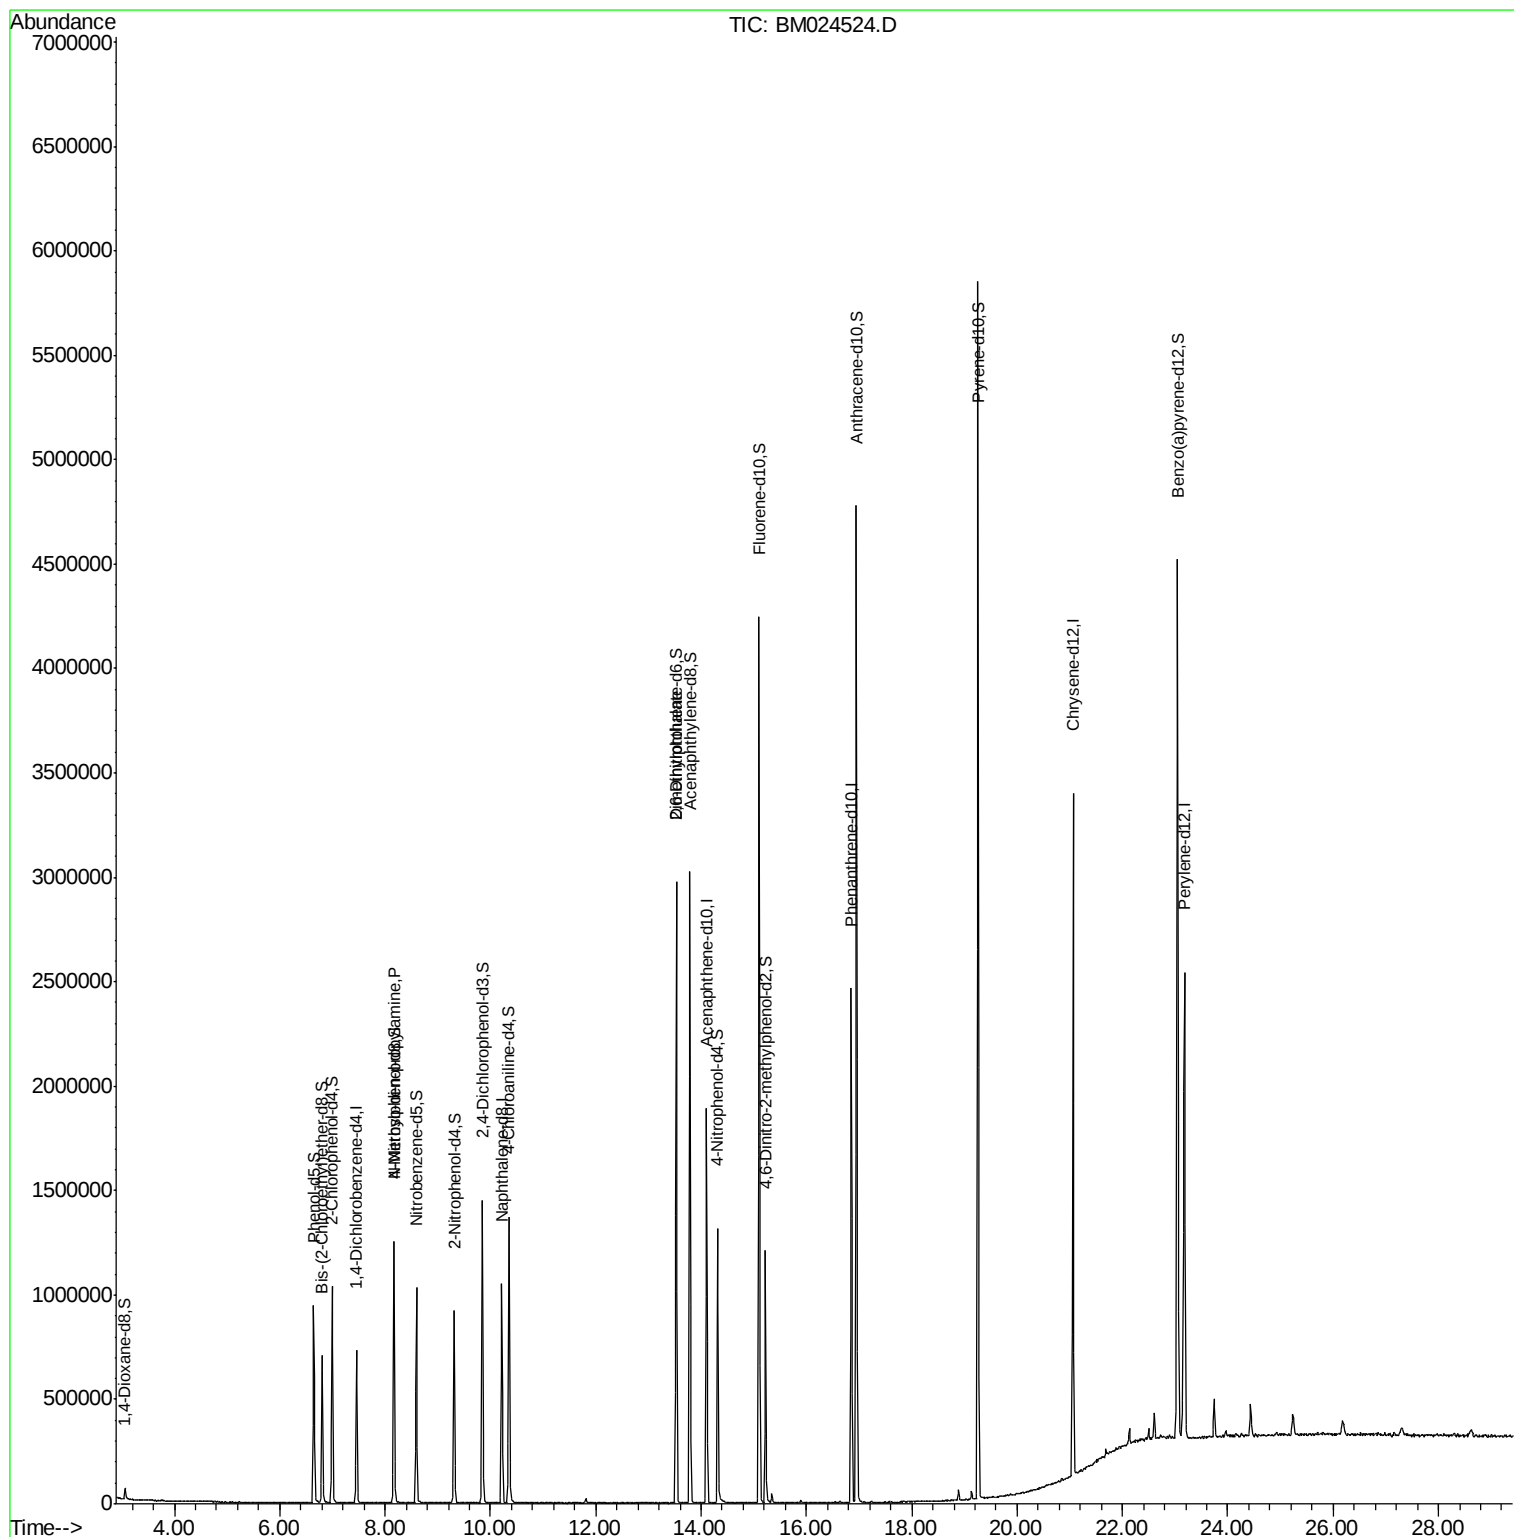

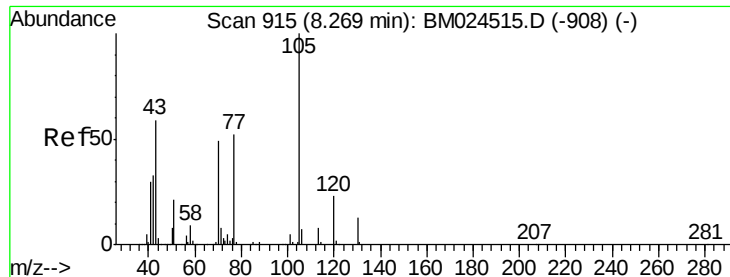

#15

N-Nitroso-di-n-propylamine

Concen: 1.136 ng/ul

RT: 8.17 min Scan# 898

Delta R.T. -0.10 min

Lab File: BM024524.D

Acq: 18 Jan 2020 08:16

Instrument :

BNA_M

ClientSampleId :

SBLK69

Tgt Ion: 70 Resp: 10878



Ion Ratio Lower Upper

70 100

42 471.4 54.1 81.1#

101 0.0 8.6 12.8#

130 0.0 19.8 29.6#

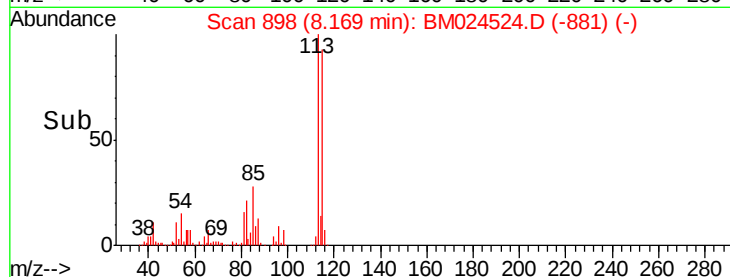
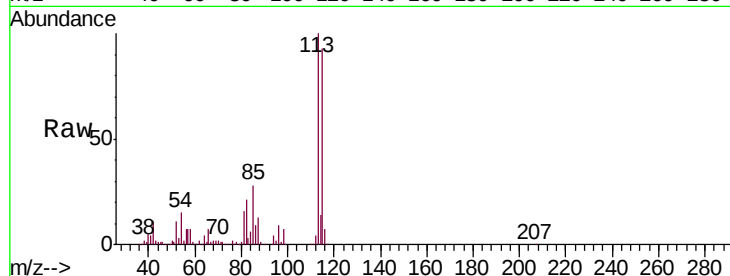


Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

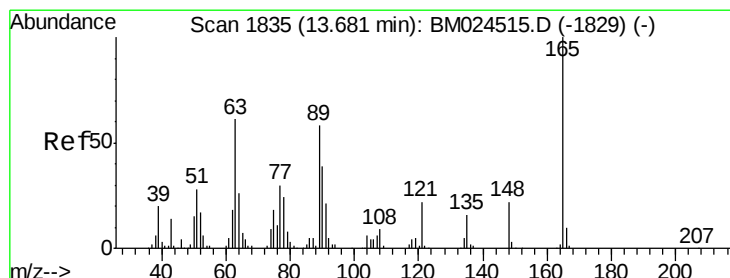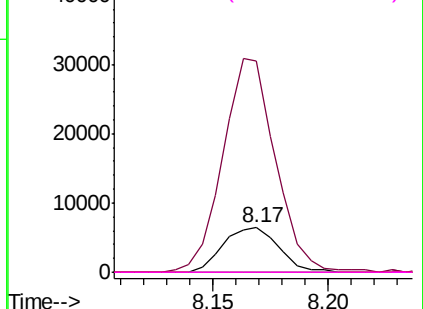

#46

2,6-Dinitrotoluene

Concen: 1.505 ng/ul

RT: 13.53 min Scan# 1809

Delta R.T. -0.15 min

Lab File: BM024524.D

Acq: 18 Jan 2020 08:16



Tgt Ion: 165 Resp: 14212

Ion Ratio Lower Upper

165 100

89 0.0 45.5 68.3#

121 30.5 17.3 25.9#

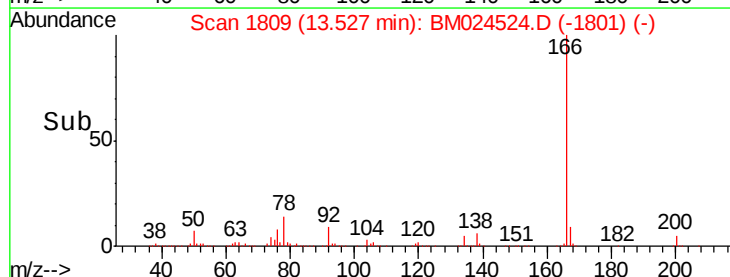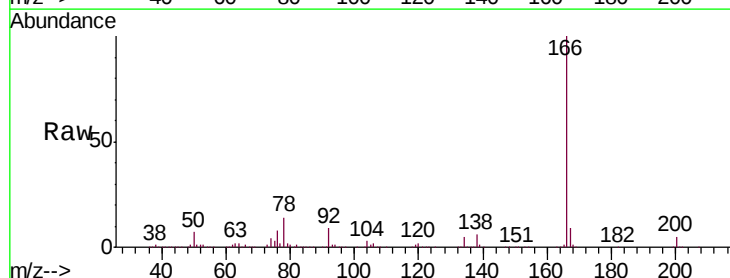

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

