

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
 Data File : BM024503.D
 Acq On : 17 Jan 2020 19:47
 Operator : JU
 Sample : L1139-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D50

Quant Time: Jan 18 00:09:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 18 00:06:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	165354	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	733795	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	547506	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	1304555	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1359778	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	1521590	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	17697	5.23	ng/uL	0.00
5) Phenol-d5	6.65	99	71472	5.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	224887	33.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	281290	26.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	162064	14.34	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	193781	37.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	217991	39.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	392530	31.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	23640	1.69	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1694100	39.49	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1887009	38.22	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	36548	5.10	ng/ul	0.00
58) Fluorene-d10	15.11	176	1463012	38.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	246620	33.12	ng/ul	0.00
71) Anthracene-d10	16.95	188	2402711	39.61	ng/ul	0.00
79) Pyrene-d10	19.26	212	2909604	40.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	3169580	40.16	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.57	163	112302	2.575	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
Data File : BM024503.D
Acq On : 17 Jan 2020 19:47
Operator : JU
Sample : L1139-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D50

Quant Time: Jan 18 00:09:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 18 00:06:51 2020
Response via : Initial Calibration

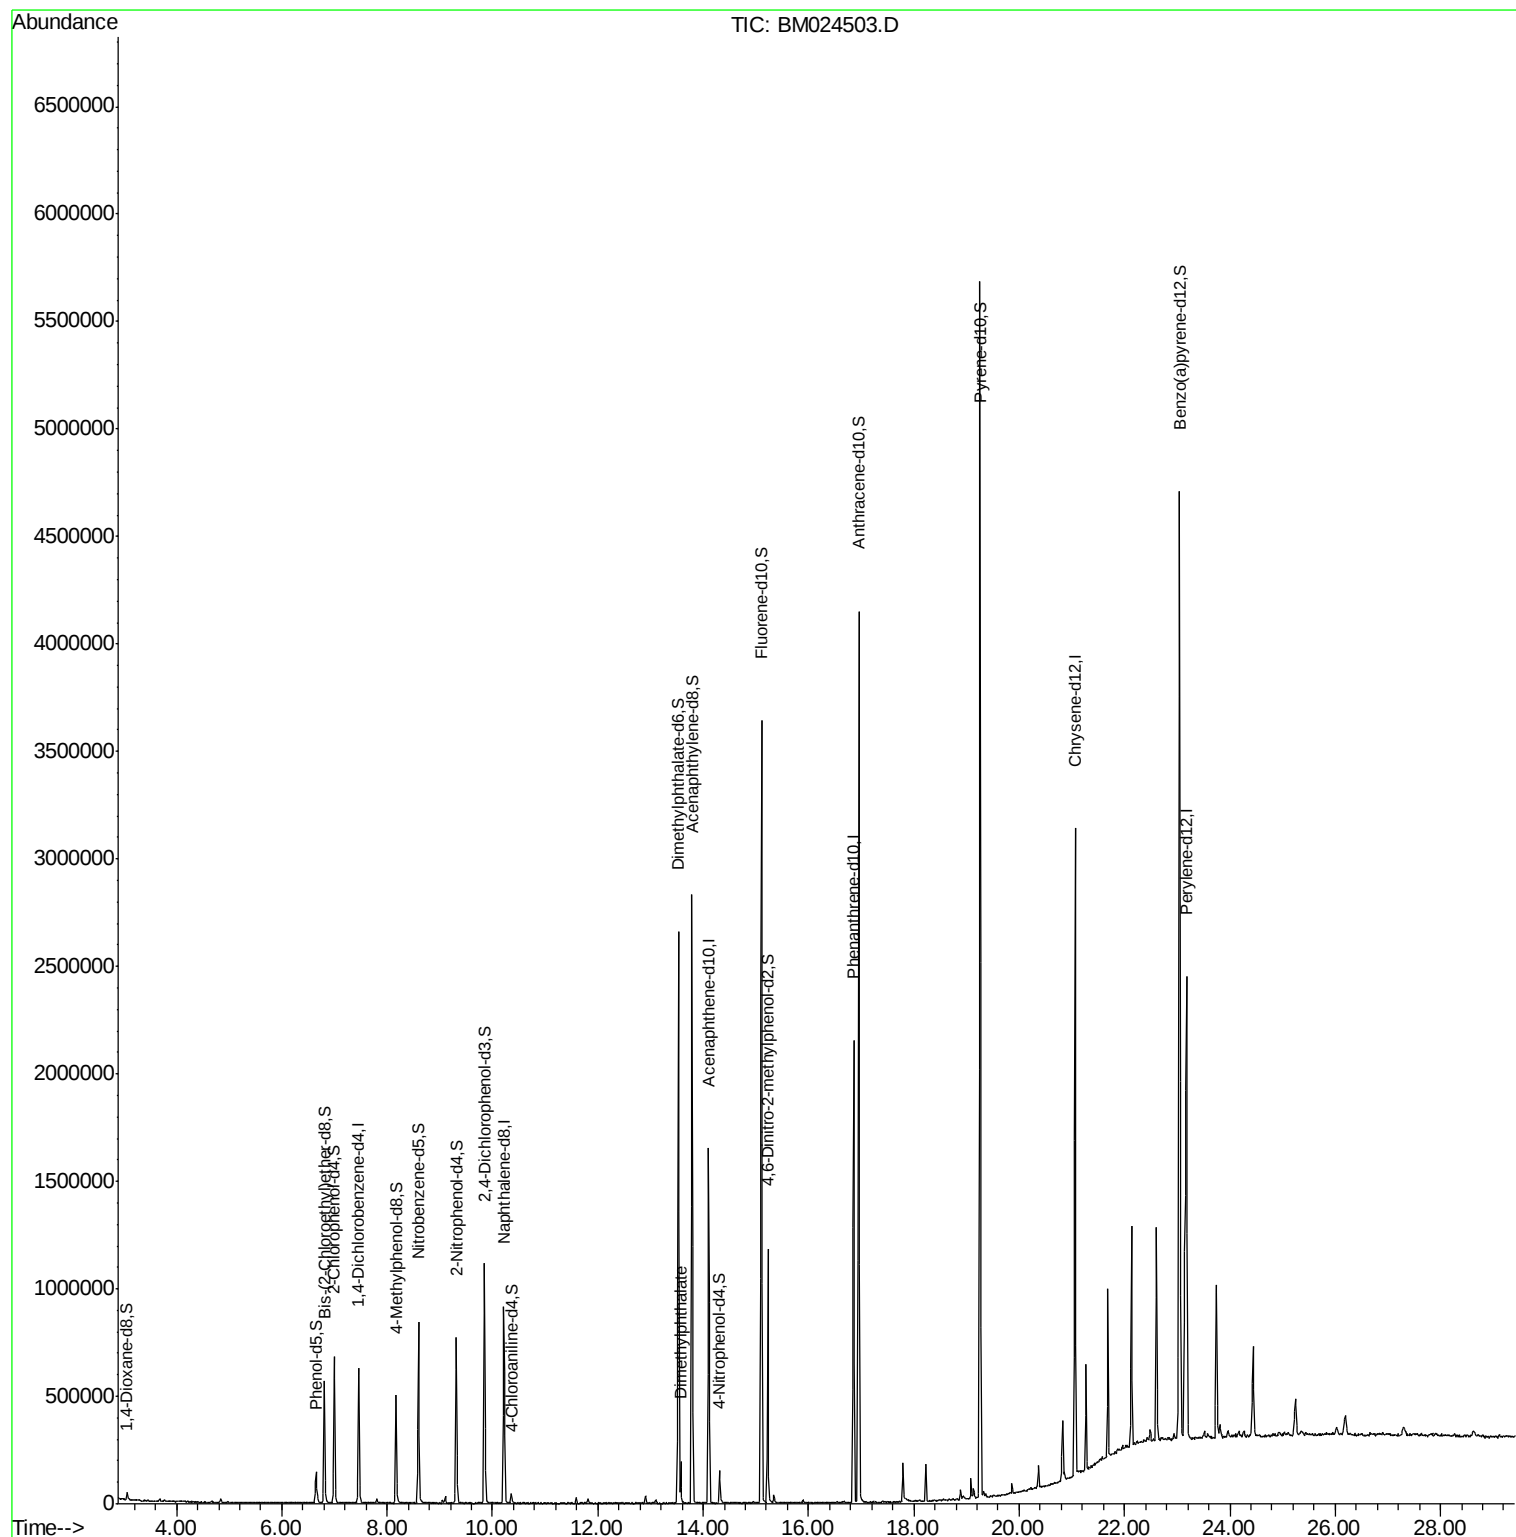

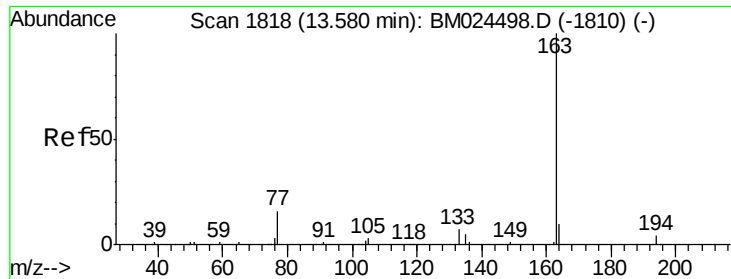

#45

Dimethylphthalate

Concen: 2.575 ng/ul

RT: 13.57 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM024503.D

Acq: 17 Jan 2020 19:47

Instrument :

BNA_M

ClientSampleId :

C0D50

Tot Ion:163 Resp: 112302

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 10.4 8.0 12.0

