

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
 Data File : BM024518.D
 Acq On : 18 Jan 2020 04:42
 Operator : JU
 Sample : L1169-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF761

Quant Time: Jan 18 05:37:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 18 05:33:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	215967	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	957301	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	710853	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1644552	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1633893	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	1632078	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	22570	5.11	ng/uL	0.00
5) Phenol-d5	6.65	99	99737	6.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	223067	25.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	300557	21.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	213453	14.46	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	190203	28.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	227804	31.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	437793	26.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	38629	2.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1757038	31.55	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1925543	30.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	54591	5.87	ng/ul	0.00
58) Fluorene-d10	15.10	176	1468572	29.95	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	274526	29.24	ng/ul	0.00
71) Anthracene-d10	16.95	188	2483530	32.47	ng/ul	0.00
79) Pyrene-d10	19.26	212	2954357	33.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	2817648	33.28	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.57	163	106756	1.886	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
Data File : BM024518.D
Acq On : 18 Jan 2020 04:42
Operator : JU
Sample : L1169-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF761

Quant Time: Jan 18 05:37:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 18 05:33:11 2020
Response via : Initial Calibration

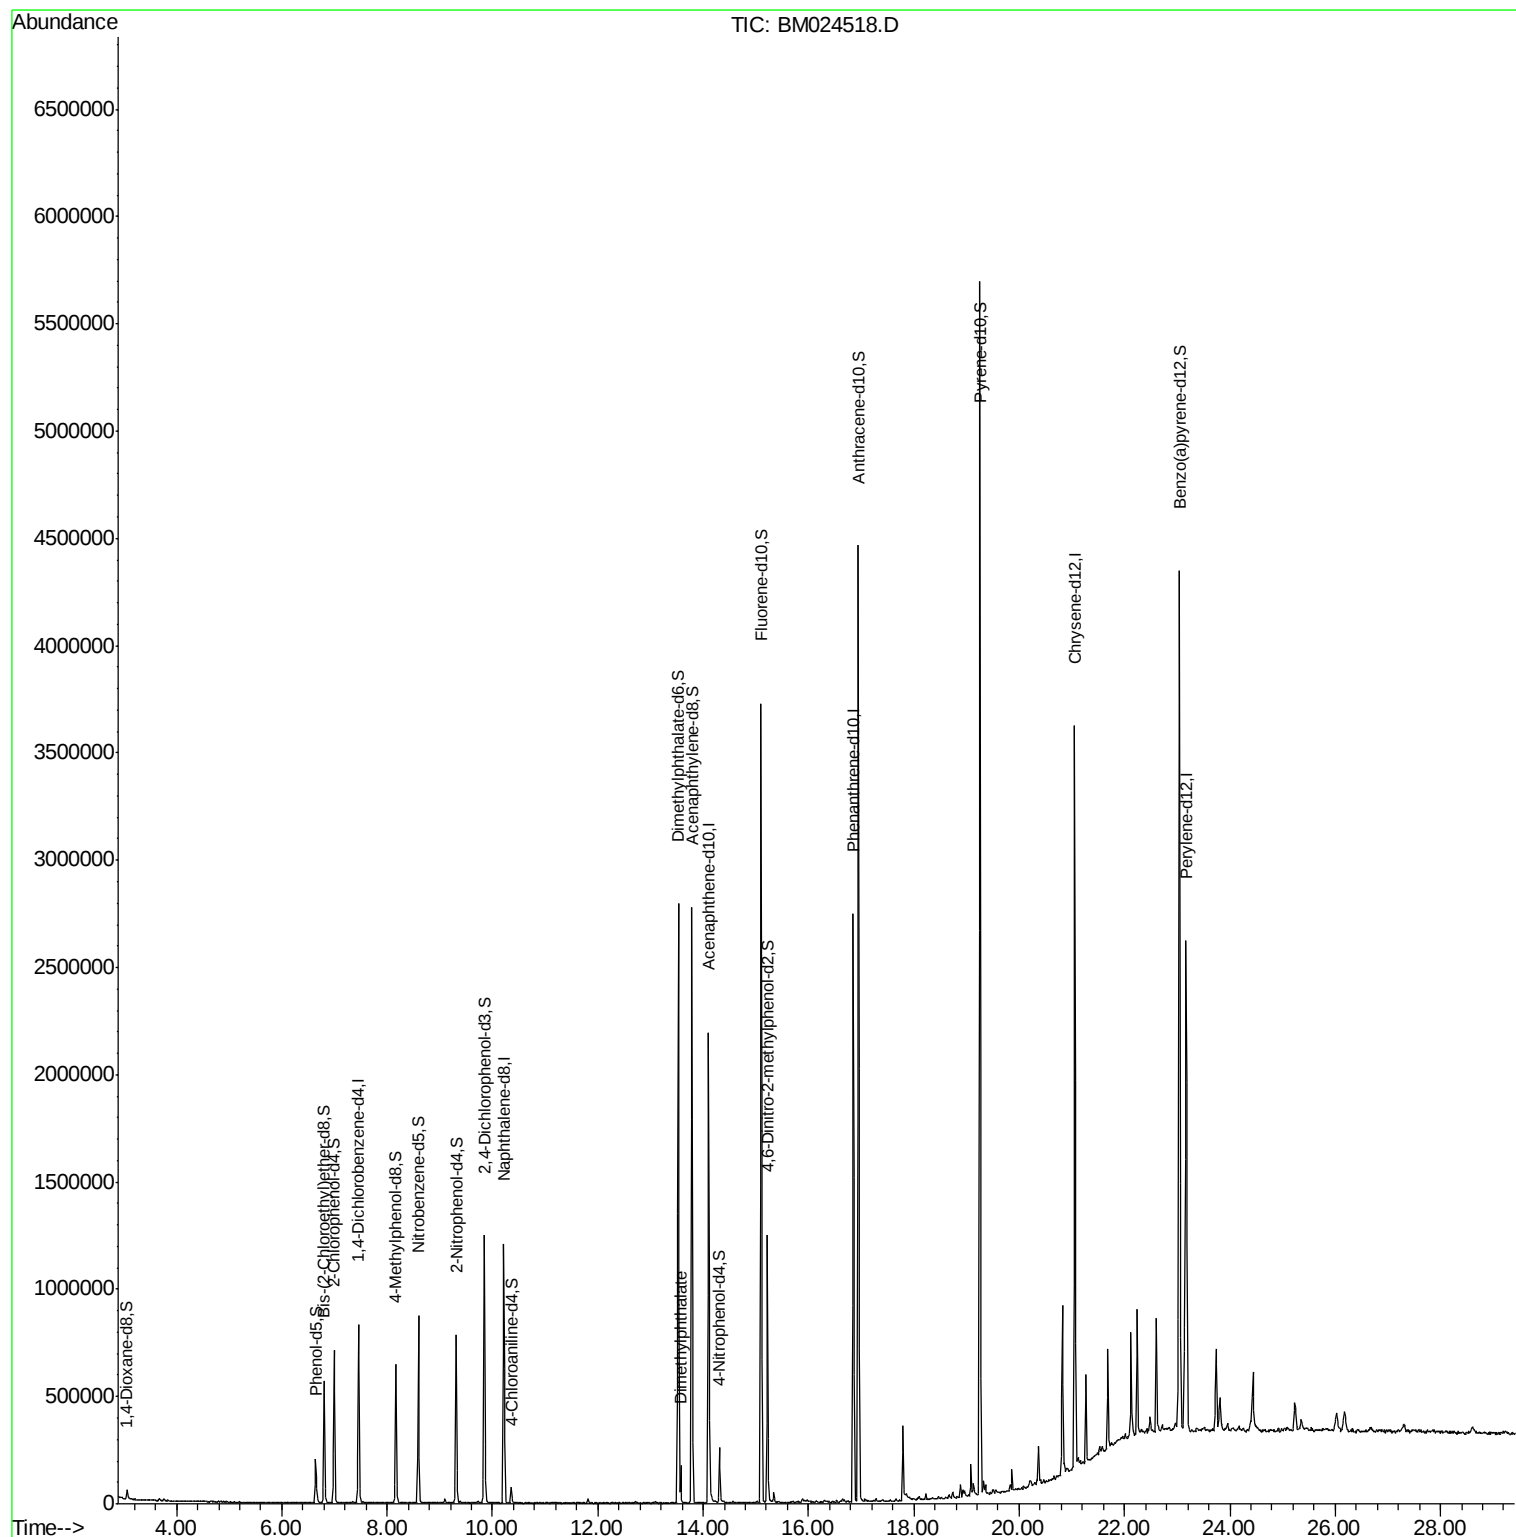

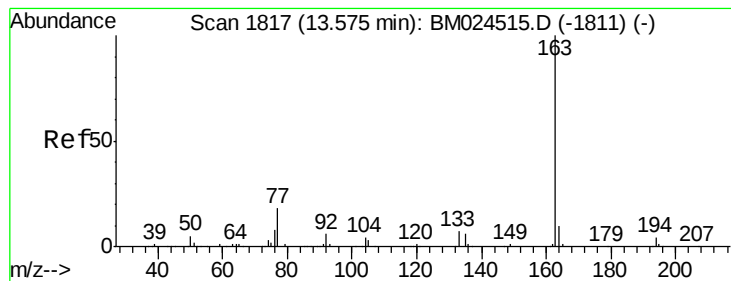

#45

Dimethylphthalate

Concen: 1.886 ng/ul

RT: 13.57 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BM024518.D

Acq: 18 Jan 2020 04:42

Instrument :

BNA_M

ClientSampleId :

BF761


Tot Ion:163 Resp: 106756

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 10.1 8.0 12.0

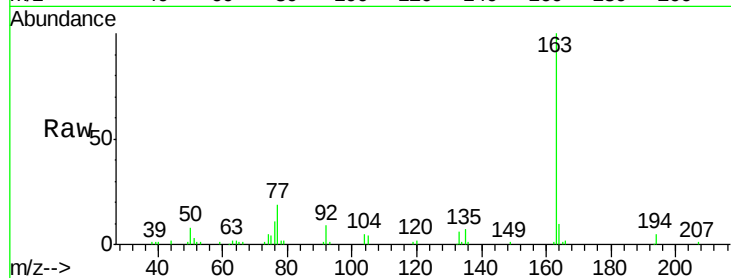

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

