

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
 Data File : BM024523.D
 Acq On : 18 Jan 2020 07:40
 Operator : JU
 Sample : L1169-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF768

Quant Time: Jan 20 01:05:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 01:02:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	221388	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	975682	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	716474	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1660489	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1762631	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	1858794	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	23431	5.17	ng/uL	0.00
5) Phenol-d5	6.65	99	116360	7.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	235337	25.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	330651	23.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	237771	15.71	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	203991	29.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	241226	32.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	476948	28.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	195392	10.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1773257	31.59	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1980387	30.65	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	62712	6.69	ng/ul	0.00
58) Fluorene-d10	15.10	176	1525596	30.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	279229	29.46	ng/ul	0.00
71) Anthracene-d10	16.95	188	2539453	32.89	ng/ul	0.00
79) Pyrene-d10	19.26	212	3027062	32.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	3152216	32.70	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.57	163	95189	1.668	ng/ul# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
Data File : BM024523.D
Acq On : 18 Jan 2020 07:40
Operator : JU
Sample : L1169-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF768

Quant Time: Jan 20 01:05:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 01:02:24 2020
Response via : Initial Calibration

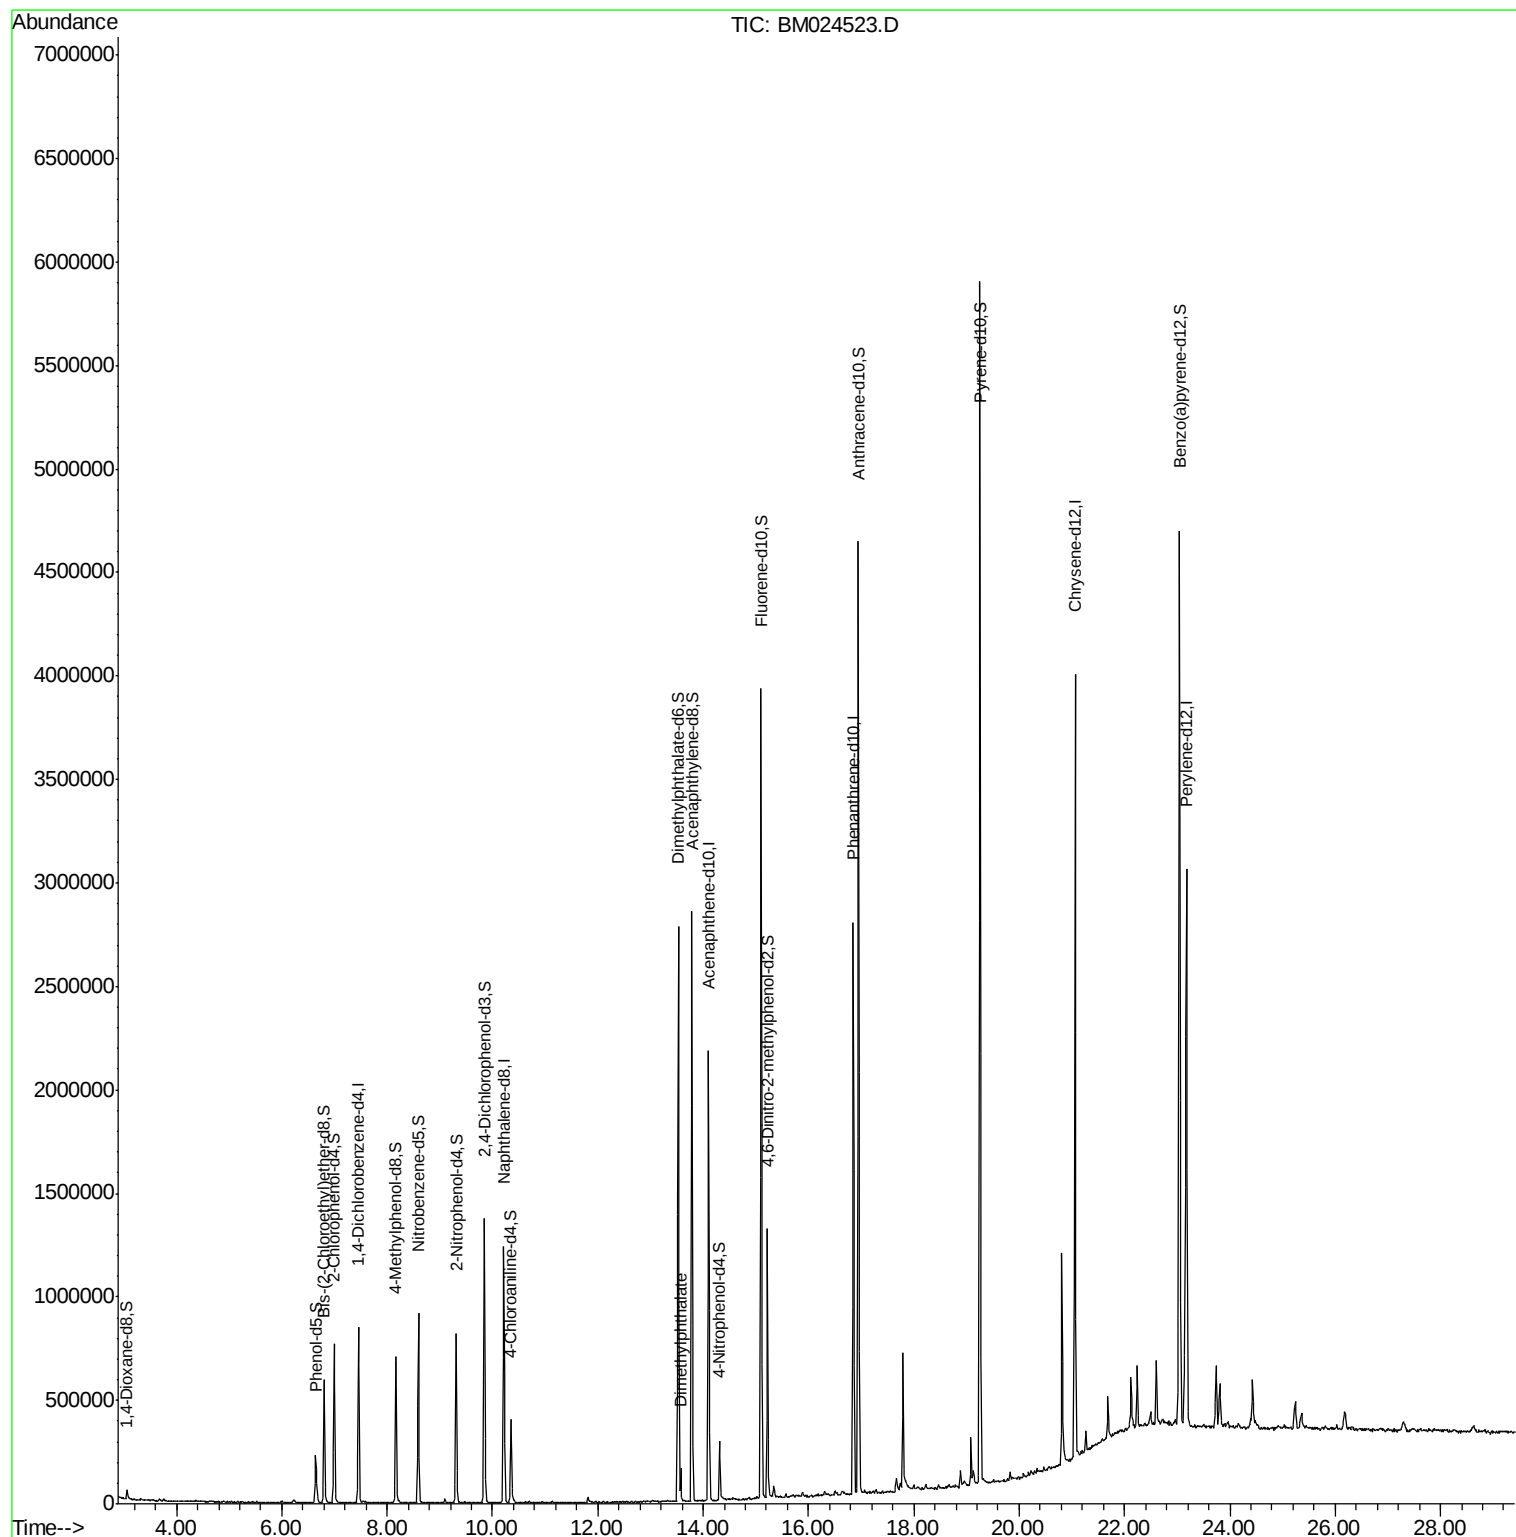

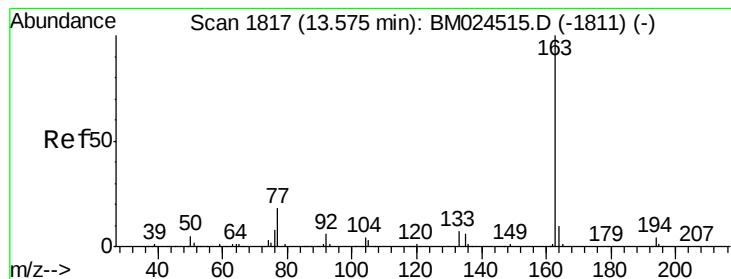

#45

Dimethylphthalate

Concen: 1.668 ng/ul

RT: 13.57 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BM024523.D

Acq: 18 Jan 2020 07:40

Instrument :

BNA_M

ClientSampleId :

BF768


Tot Ion:163 Resp: 95189

Ion Ratio Lower Upper

163 100

194 5.1 3.4 5.0#

164 10.9 8.0 12.0

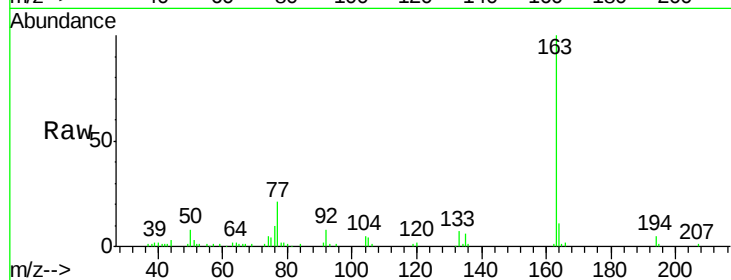

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

