

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
 Data File : BM024528.D
 Acq On : 18 Jan 2020 10:39
 Operator : JU
 Sample : L1169-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF774

Quant Time: Jan 20 01:05:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 01:02:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	255286	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	1117649	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	822261	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1905537	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1823371	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	1750463	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	27421	5.25	ng/uL	0.00
5) Phenol-d5	6.65	99	127464	6.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	283134	26.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	382593	23.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	272529	15.62	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	244708	31.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	289725	34.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	560400	29.28	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	45228	2.13	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	2313038	35.90	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	2496202	33.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	72152	6.71	ng/ul	0.00
58) Fluorene-d10	15.10	176	1931726	34.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	359875	33.08	ng/ul	0.00
71) Anthracene-d10	16.95	188	3199984	36.11	ng/ul	0.00
79) Pyrene-d10	19.26	212	3802578	39.02	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.05	264	3401087	37.46	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.57	163	98312	1.501	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
Data File : BM024528.D
Acq On : 18 Jan 2020 10:39
Operator : JU
Sample : L1169-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF774

Quant Time: Jan 20 01:05:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 01:02:24 2020
Response via : Initial Calibration

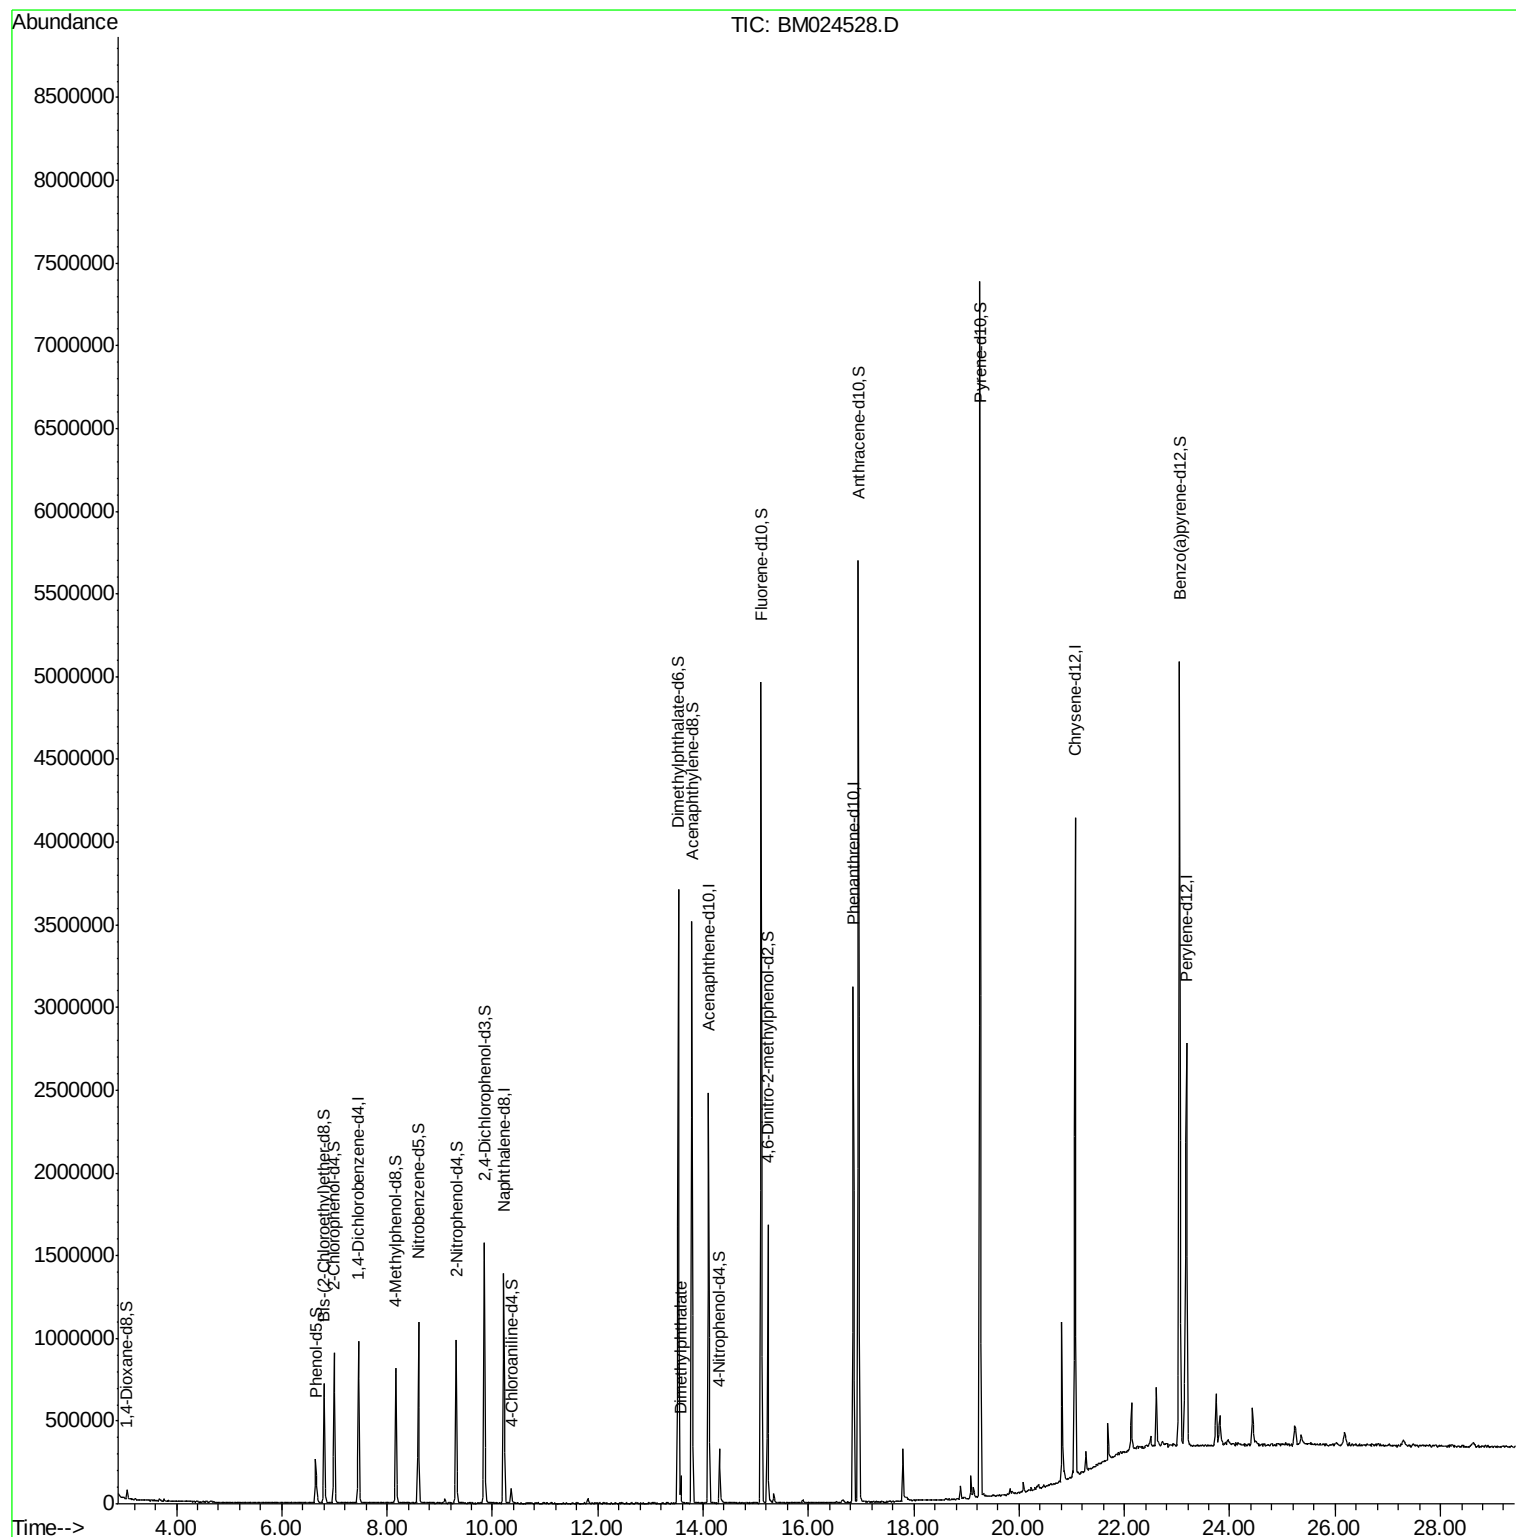

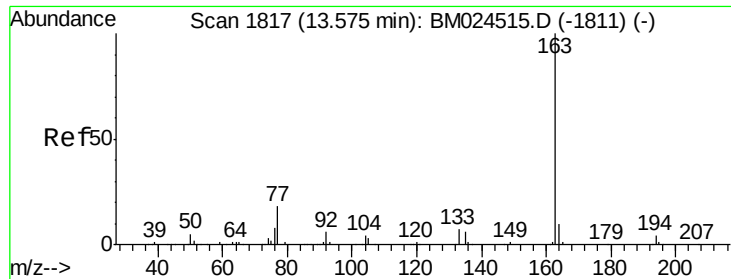

#45

Dimethylphthalate

Concen: 1.501 ng/ul

RT: 13.57 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BM024528.D

Acq: 18 Jan 2020 10:39

Instrument :

BNA_M

ClientSampleId :

BF774


Tot Ion:163 Resp: 98312

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 9.9 8.0 12.0

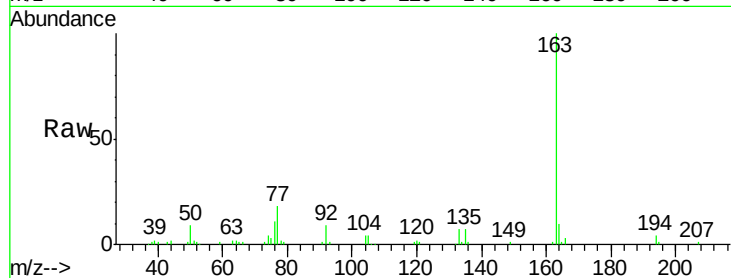

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

