

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
 Data File : BM024530.D
 Acq On : 18 Jan 2020 11:50
 Operator : JU
 Sample : L1169-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF777

Quant Time: Jan 20 01:06:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 01:02:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	206038	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	905485	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	682988	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1610828	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1560455	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	1524367	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	19525	4.63	ng/uL	0.00
5) Phenol-d5	6.65	99	88318	5.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	218491	25.76	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	287183	22.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	191663	13.61	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	187521	29.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	214867	31.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	397937	25.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	34765	2.02	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1745730	32.62	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1879648	30.52	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	51686	5.79	ng/ul	0.00
58) Fluorene-d10	15.10	176	1517981	32.22	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	261151	28.40	ng/ul	0.00
71) Anthracene-d10	16.95	188	2581305	34.46	ng/ul	0.00
79) Pyrene-d10	19.26	212	3004834	36.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	2721950	34.43	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.57	163	70292	1.292	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
Data File : BM024530.D
Acq On : 18 Jan 2020 11:50
Operator : JU
Sample : L1169-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF777

Quant Time: Jan 20 01:06:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 01:02:24 2020
Response via : Initial Calibration

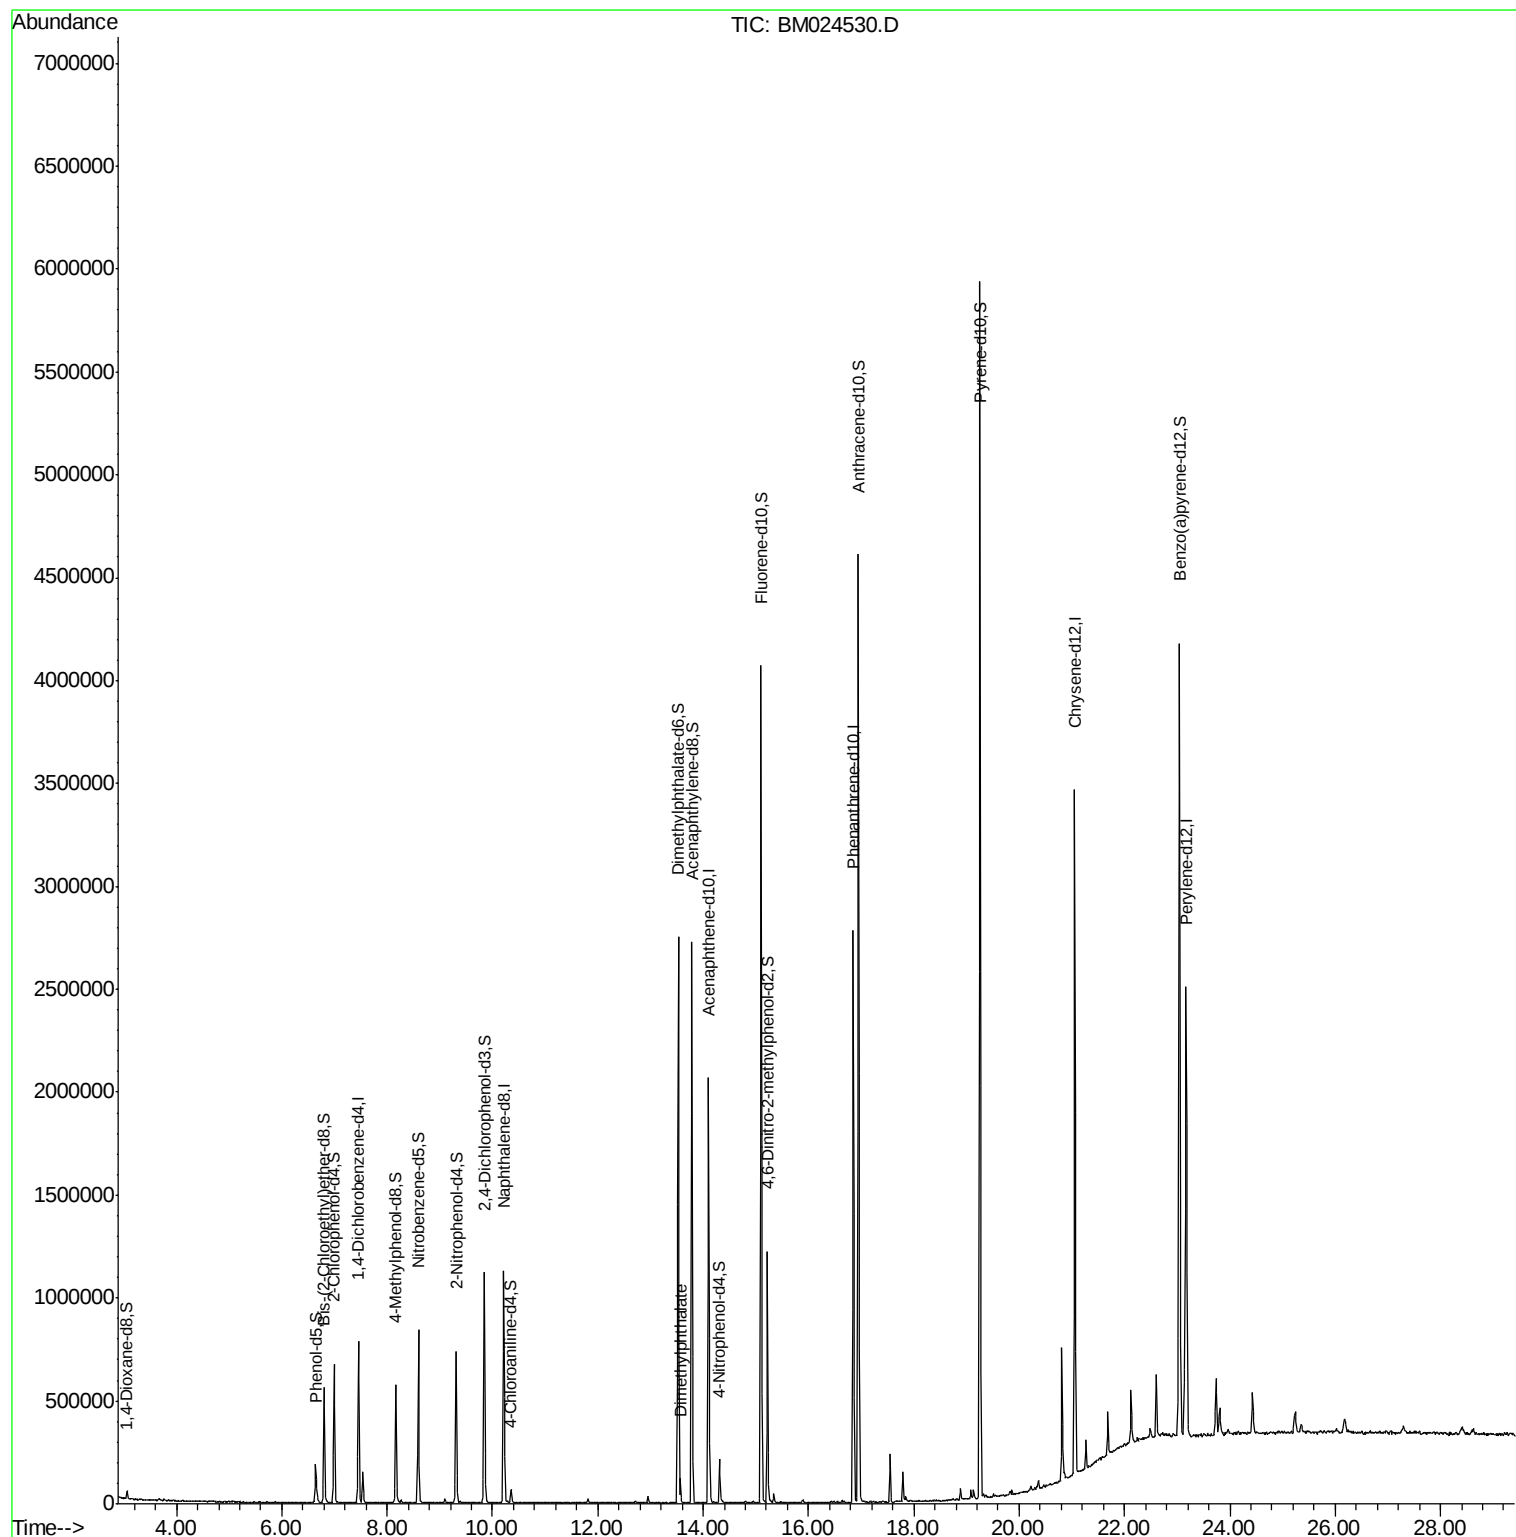


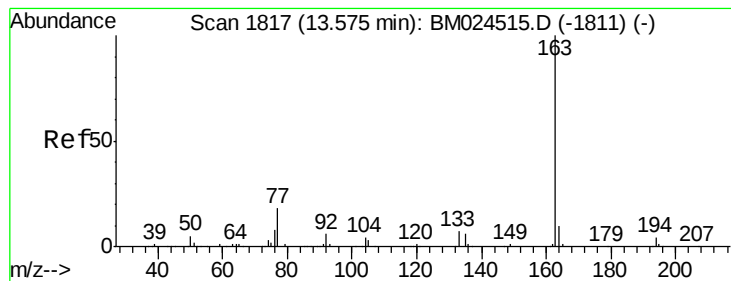

#45
 Dimethylphthalate
 Concen: 1.292 ng/ul
 RT: 13.57 min Scan# 1817
 Delta R.T. -0.00 min
 Lab File: BM024530.D
 Acq: 18 Jan 2020 11:50

Instrument :
 BNA_M
 ClientSampleId :
 BF777

Tot Ion:163 Resp: 70292
 Ion Ratio Lower Upper
 163 100
 194 3.8 3.4 5.0
 164 9.9 8.0 12.0

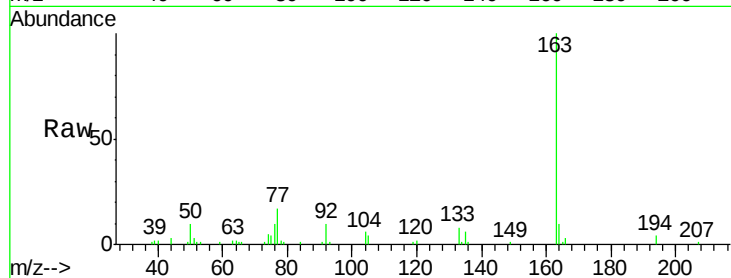

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

