

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
 Data File : BM024541.D
 Acq On : 18 Jan 2020 18:22
 Operator : JU
 Sample : L1109-02MS
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GASG2MS

Manual Integrations
 APPROVED

mohammad
 1/21/2020 8:00:04 AM

Quant Time: Jan 20 06:05:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 03:25:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	214249	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	964716	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	671422	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	1464812	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1544453	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1643170	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	11245	2.56	ng/uL	0.00
5) Phenol-d5	6.65	99	273445	17.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	162457	18.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	253882	18.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	231125	15.78	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	135216	19.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	161280	21.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	293902	17.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	288543	15.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1077690	20.48	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1192705	19.70	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	193835	22.08	ng/ul	0.00
58) Fluorene-d10	15.10	176	926708	20.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	154213	18.44	ng/ul	0.00
71) Anthracene-d10	16.96	188	1494965	21.95	ng/ul	0.00
79) Pyrene-d10	19.26	212	1769121	21.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	1869132	21.93	ng/ul	0.01

Target Compounds

					Ovalue	
6) Phenol	6.67	94	331382	20.535	ng/ul	93
10) 2-Chlorophenol	7.03	128	273976	20.184	ng/ul	99
15) N-Nitroso-di-n-propylamine	8.26	70	227770	20.960	ng/ul	94
33) 4-Chloro-3-methylphenol	11.52	107	347265	20.842	ng/ul	97
45) Dimethylphthalate	13.57	163	276348	5.167	ng/ul	99
48) Acenaphthylene	13.82	152	172438	2.788	ng/ul	97
50) Acenaphthene	14.17	153	859271	20.527	ng/ul	99
53) 4-Nitrophenol	14.33	109	194101	23.773	ng/ul	96
54) Dibenzofuran	14.51	168	103264	1.684	ng/ul	98
55) 2,4-Dinitrotoluene	14.48	165	369079	24.530	ng/ul	94
59) Fluorene	15.16	166	116546	2.248	ng/ul	97
69) Pentachlorophenol	16.52	266	262065	22.072	ng/ul	99
70) Phenanthrene	16.90	178	1295381	16.398	ng/ul	100
72) Anthracene	16.99	178	356293	4.423	ng/ul	98
77) Fluoranthene	18.93	202	1409376	14.597	ng/ul	100
80) Pyrene	19.29	202	3735982	35.335	ng/ul	99
83) Benzo(a)anthracene	21.05	228	800833m	7.612	ng/ul	
85) Chrysene	21.10	228	716032	7.063	ng/ul	99
88) Benzo(b)fluoranthene	22.57	252	691769	6.370	ng/ul	99
89) Benzo(k)fluoranthene	22.60	252	251203m	2.354	ng/ul	
91) Benzo(a)pyrene	23.10	252	543991	5.764	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.26	276	281346	2.849	ng/ul	98
93) Dibenz(a,h)anthracene	25.26	278	92143	1.099	ng/ul#	95

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
Data File : BM024541.D
Acq On : 18 Jan 2020 18:22
Operator : JU
Sample : L1109-02MS
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG2MS

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

Quant Time: Jan 20 06:05:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
94) Benzo(q,h,i)perylene	25.89	276	197764	2.520	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011720\
Data File : BM024541.D
Acq On : 18 Jan 2020 18:22
Operator : JU
Sample : L1109-02MS
Misc :
ALS Vial : 45 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
GASG2MS

Quant Time: Jan 20 06:05:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 03:25:57 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

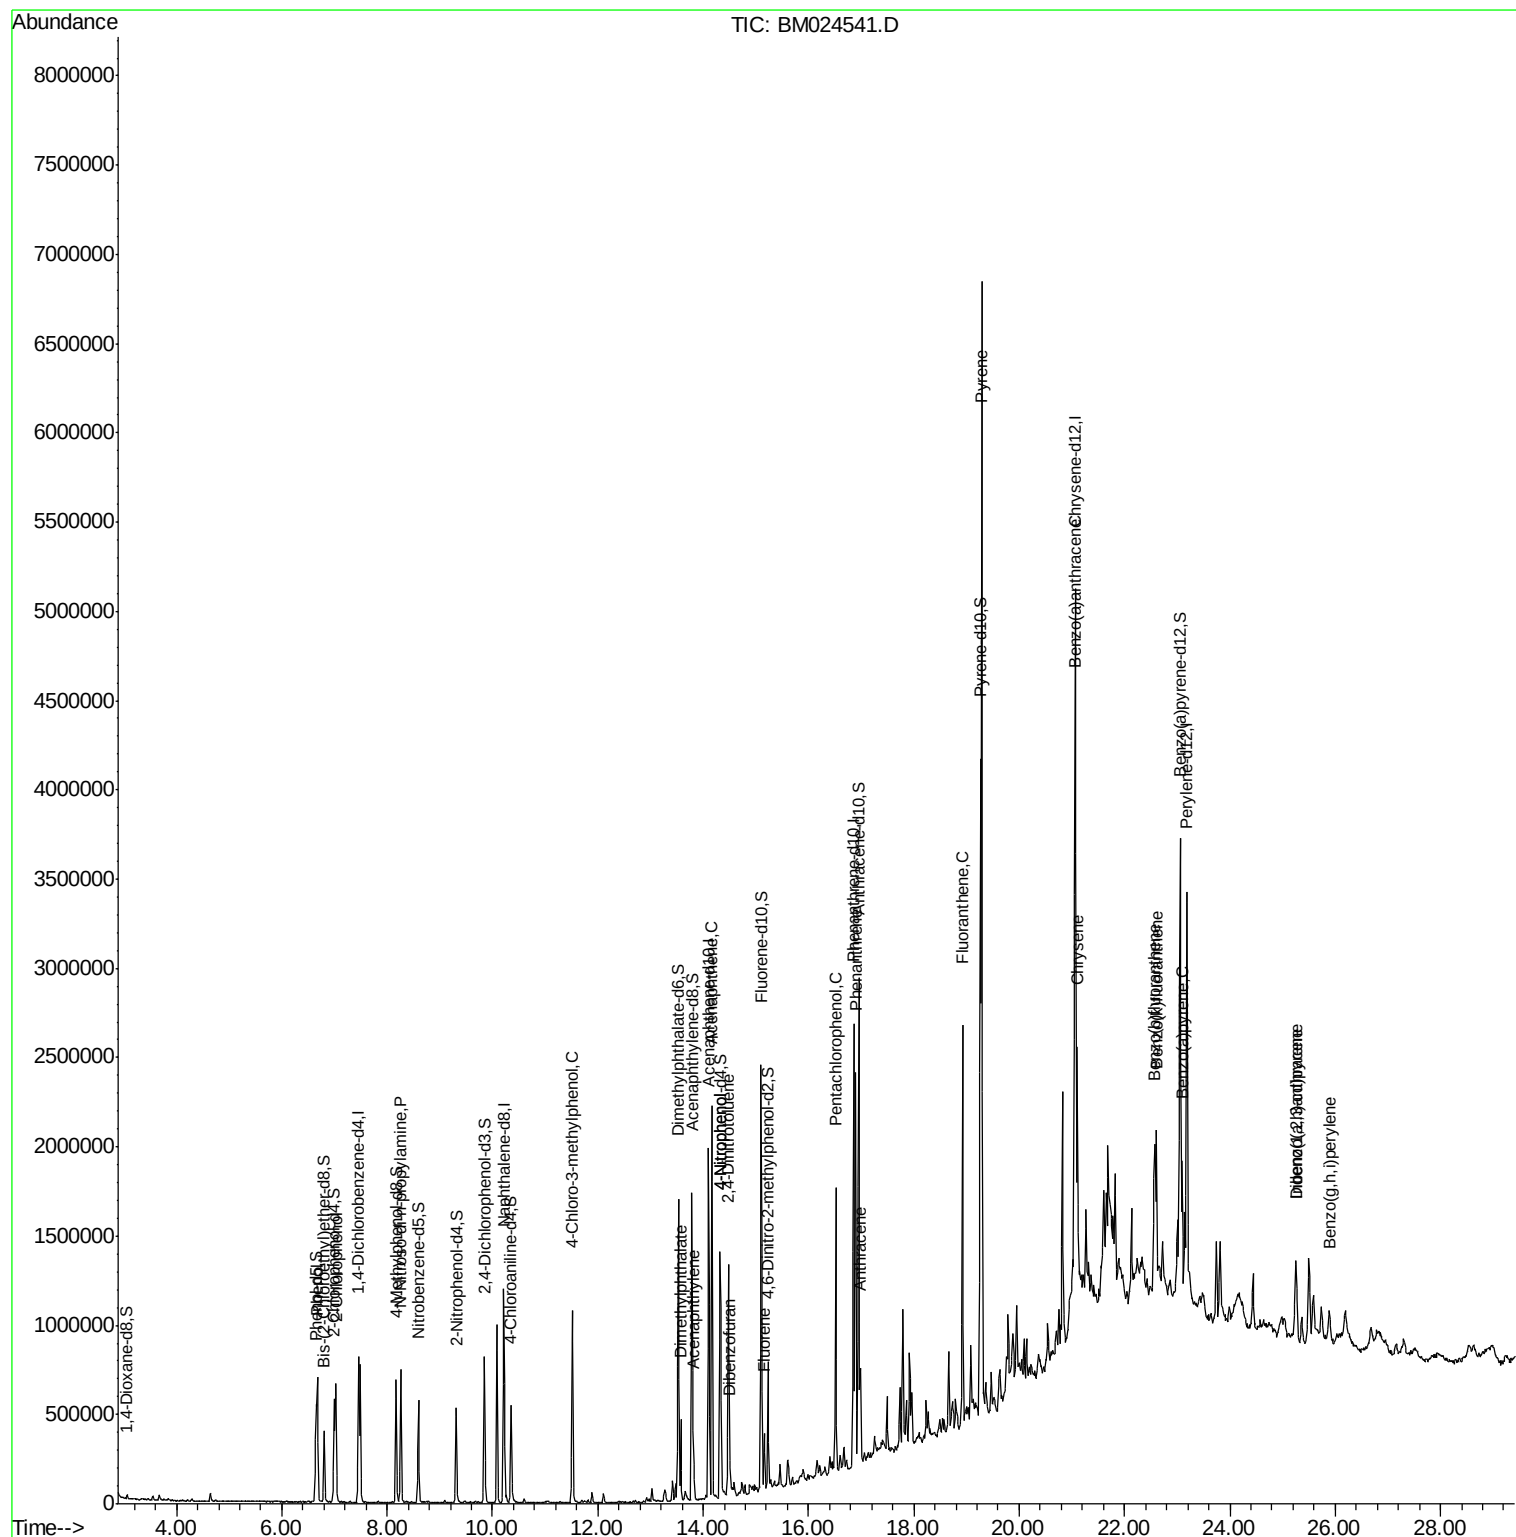

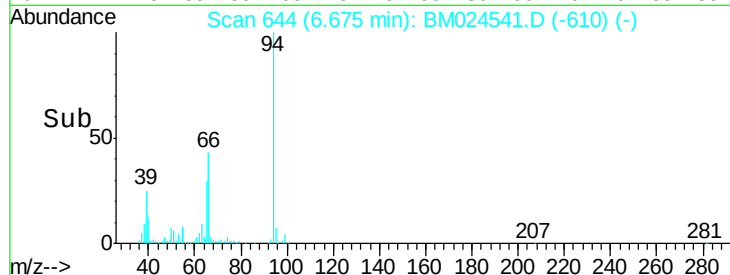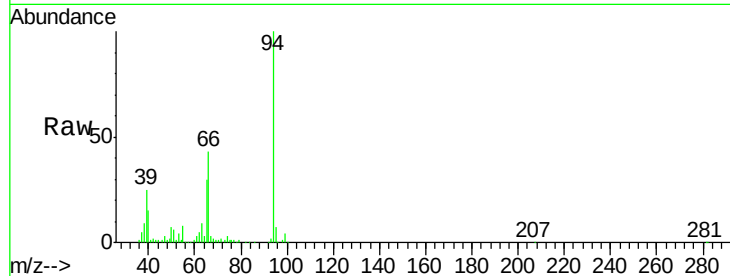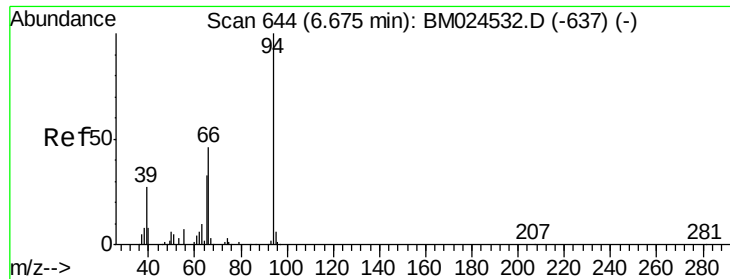

#6

Phenol





Concen: 20.535 ng/ul
RT: 6.67 min Scan# 644
Delta R.T. -0.00 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Tot Ion	Ratio	Resp	Lower	Upper
94	100			
65	30.3	26.7	40.1	
66	42.7	38.1	57.1	

Instrument :
BNA_M
ClientSampleId :
GASG2MS

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

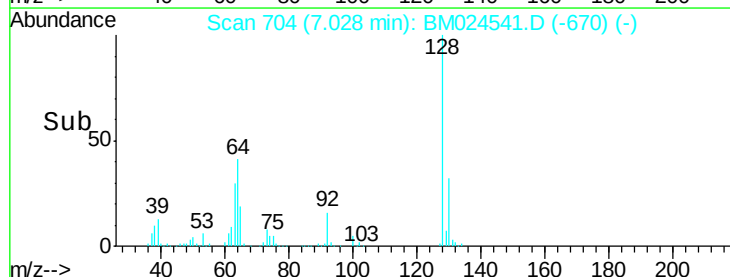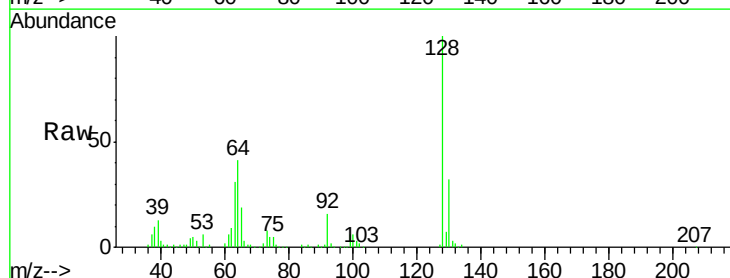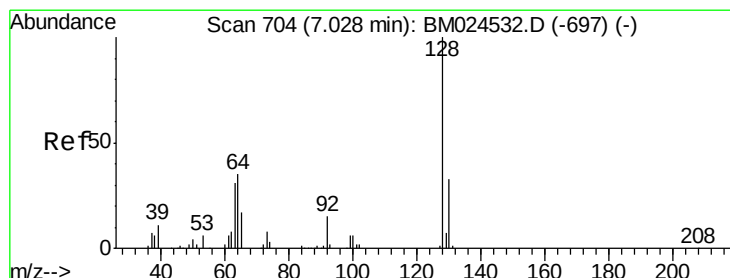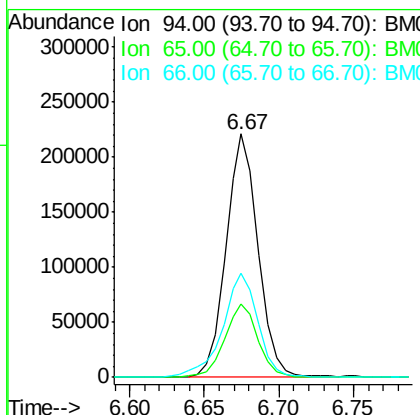



#10

2-Chlorophenol

Concen: 20.184 ng/ul
RT: 7.03 min Scan# 704
Delta R.T. -0.00 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Tgt Ion	Ratio	Resp	Lower	Upper
128	100			
64	41.1	34.0	51.0	
130	31.7	25.4	38.2	

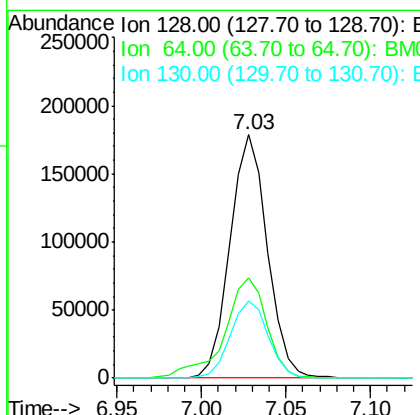

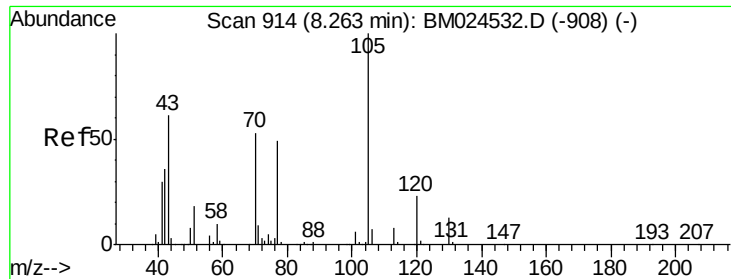





#15
N-Nitroso-di-n-propylamine
Concen: 20.960 ng/ul
RT: 8.26 min Scan# 914
Delta R.T. -0.00 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Instrument :
BNA_M
ClientSampleId :
GAS2MS

Tot Ion	Ratio	Lower	Upper
70	100		
42	60.8	54.1	81.1
101	10.7	8.6	12.8
130	23.9	19.8	29.6




Manual Integrations
APPROVED


mohammad
1/21/2020 8:00:04 AM

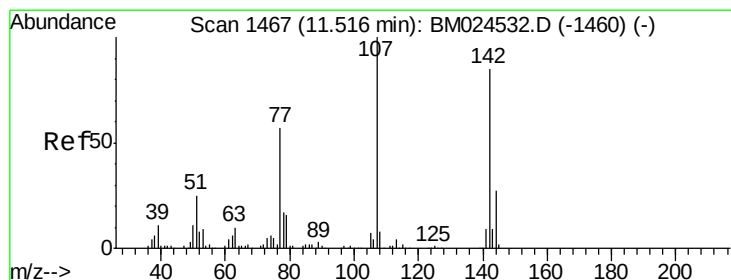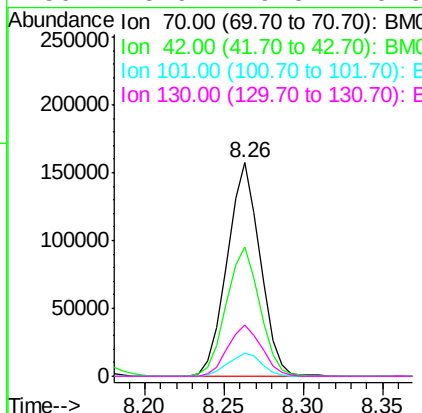

#33
4-Chloro-3-methylphenol
Concen: 20.842 ng/ul
RT: 11.52 min Scan# 1467
Delta R.T. -0.00 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Tgt Ion	Ratio	Lower	Upper
107	100		
144	27.7	21.3	31.9
142	83.0	68.7	103.1

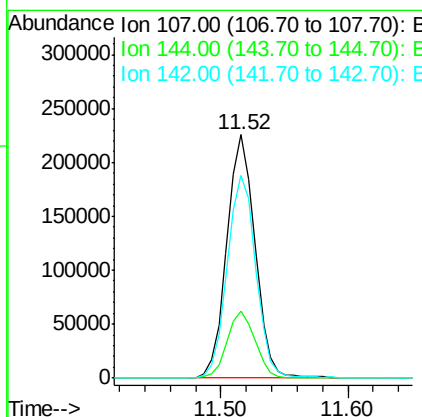

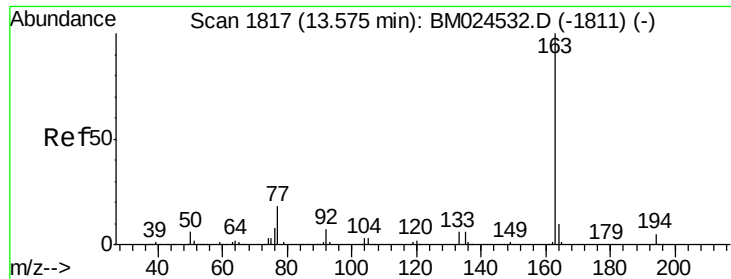





#45
Dimethylphthalate
Concen: 5.167 ng/ul
RT: 13.57 min Scan# 1817
Delta R.T. -0.00 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Instrument :
BNA_M
ClientSampleId :
GASG2MS

Tot Ion	Ratio	Resp	Lower	Upper
163	100	276348		
194	4.0		3.4	5.0
164	10.3		8.0	12.0




Manual Integrations
APPROVED


mohammad
1/21/2020 8:00:04 AM

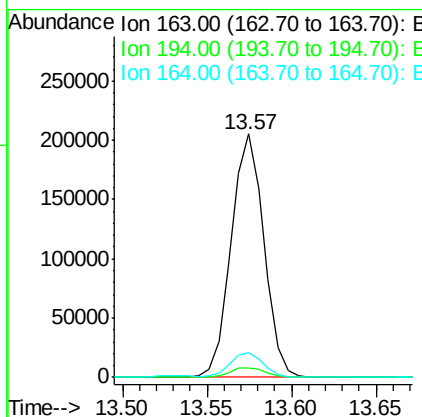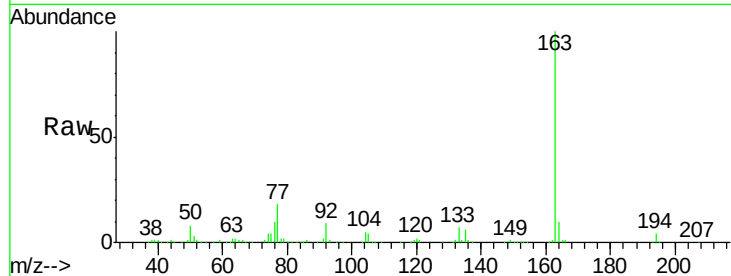

#48
Acenaphthylene
Concen: 2.788 ng/ul
RT: 13.82 min Scan# 1858
Delta R.T. -0.00 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	172438		
151	19.2		15.9	23.9
153	14.7		10.3	15.5

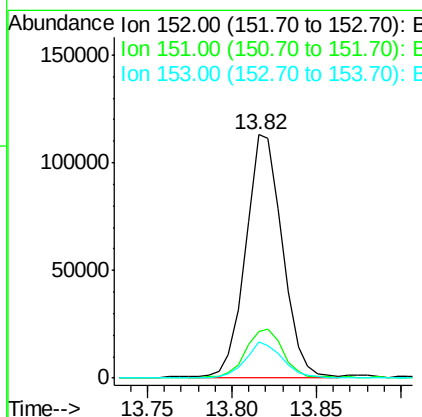

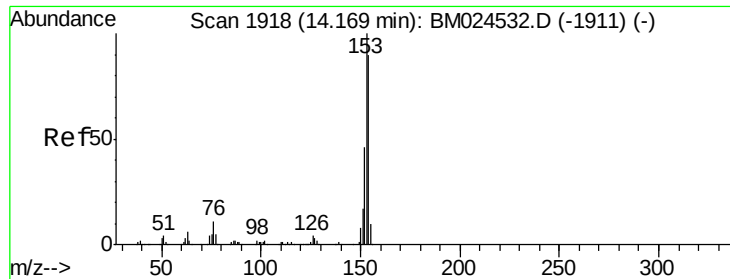

#50

Acenaphthene

Concen: 20.527 ng/ul

RT: 14.17 min Scan# 1918

Delta R.T. -0.00 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Instrument :

BNA_M


ClientSampleId :

GASG2MS




Tot Ion:	153	Resp:	859271
Ion Ratio	Lower	Upper	
153	100		
152	45.9	37.2	55.8
154	89.2	70.6	106.0

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

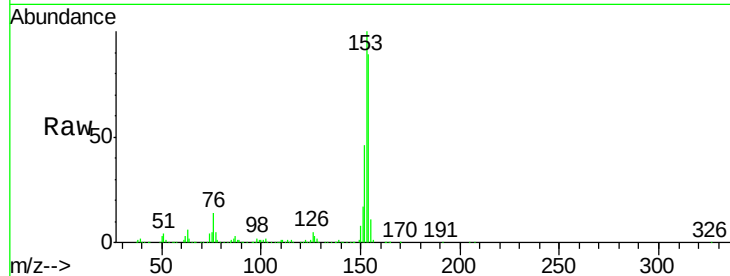

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

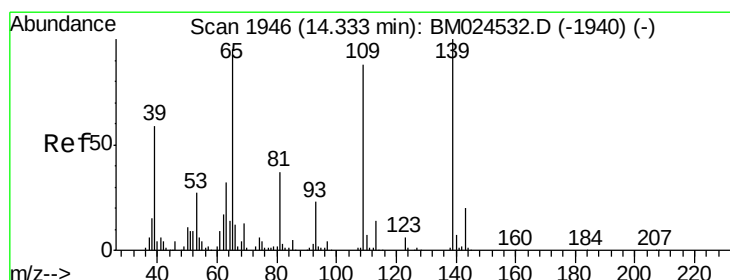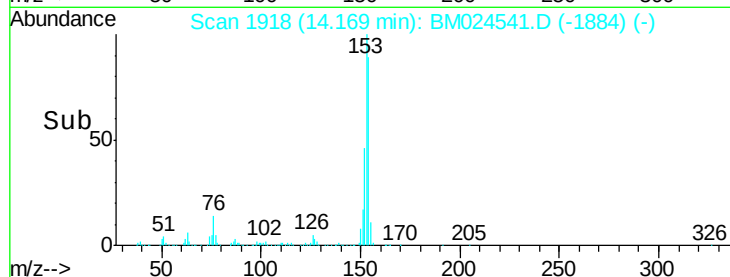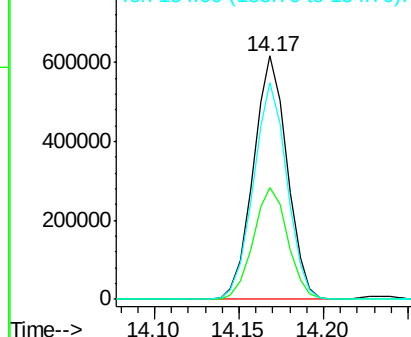

#53

4-Nitrophenol

Concen: 23.773 ng/ul


RT: 14.33 min Scan# 1946

Delta R.T. -0.00 min



Lab File: BM024541.D




Acq: 18 Jan 2020 18:22

Tgt Ion:	109	Resp:	194101
Ion Ratio	Lower	Upper	
109	100		
139	118.7	88.6	133.0
65	116.0	91.8	137.8

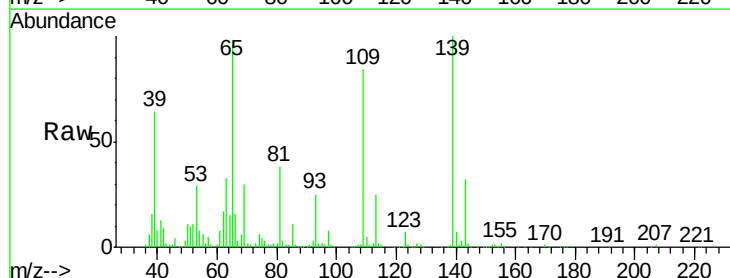

Abundance Ion 109.00 (108.70 to 109.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 65.00 (64.70 to 65.70): BM

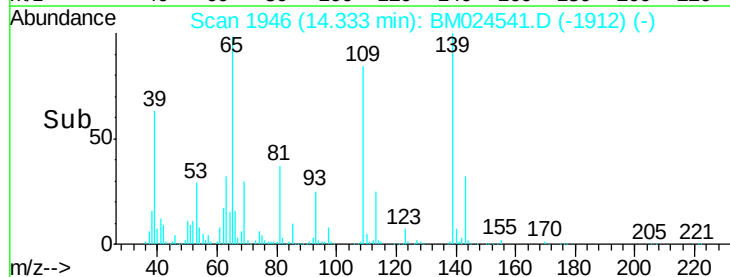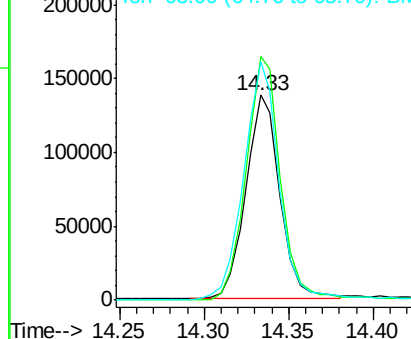

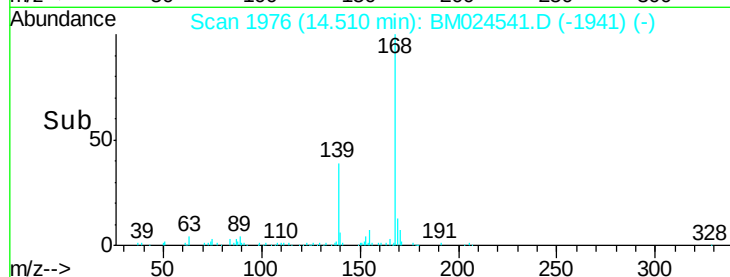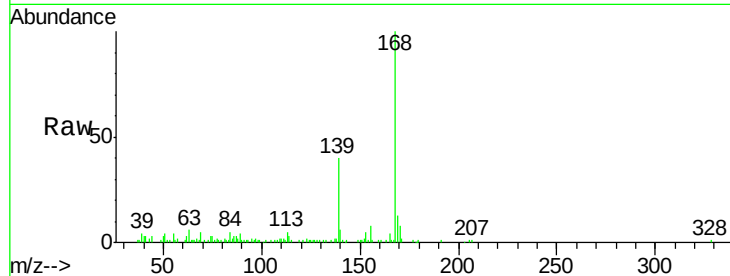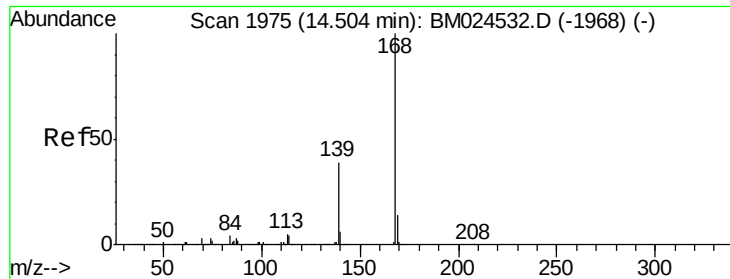

#54

Dibenzofuran

Concen: 1.684 ng/ul

RT: 14.51 min Scan# 1976

Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Tot Ion:168 Resp: 103264

Ion Ratio Lower Upper

168 100

139 39.9 30.7 46.1

Instrument :

BNA_M

ClientSampleId :





GAS2MS

Manual Integrations

APPROVED

mohammad

1/21/2020 8:00:04 AM

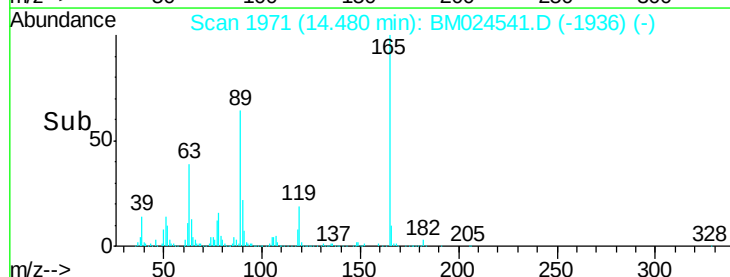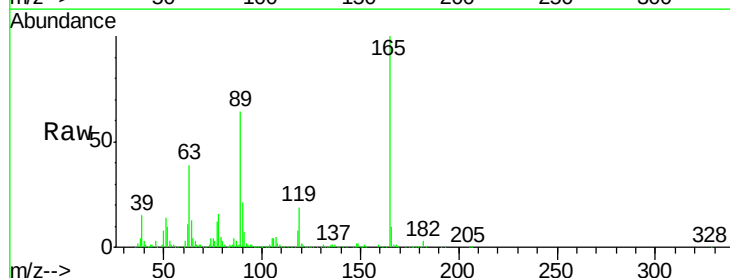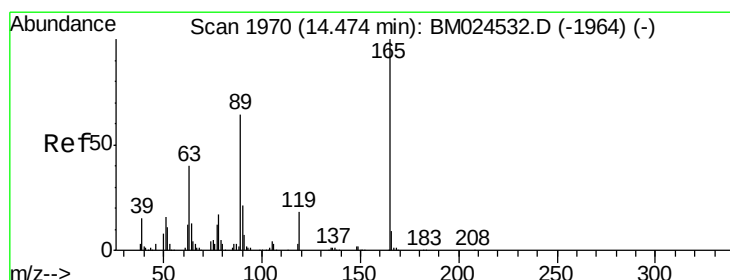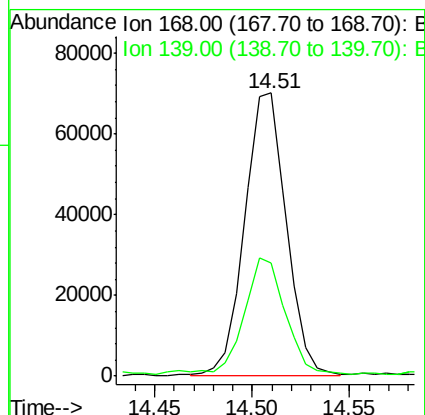

#55

2,4-Dinitrotoluene

Concen: 24.530 ng/ul

RT: 14.48 min Scan# 1971

Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22


Tgt Ion:165 Resp: 369079


Ion Ratio Lower Upper

165 100

63 38.9 34.4 51.6

182 3.1 2.2 3.2

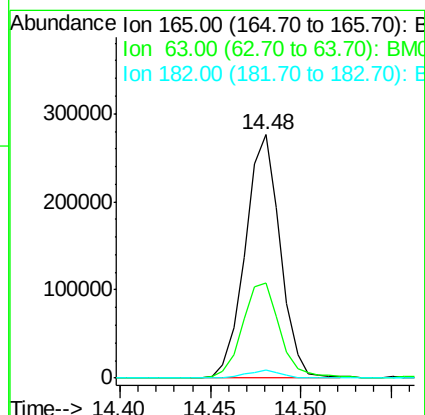

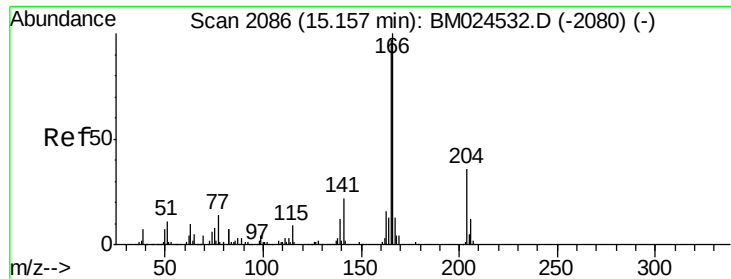





#59
Fluorene
Concen: 2.248 ng/ul
RT: 15.16 min Scan# 2087
Delta R.T. 0.01 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Instrument :
BNA_M
ClientSampled :
GAS2MS

Tot Ion	Ratio	Resp	Lower	Upper
166	100			
165	102.6	79.6	119.4	
167	14.4	10.8	16.2	




Manual Integrations
APPROVED


mohammad
1/21/2020 8:00:04 AM

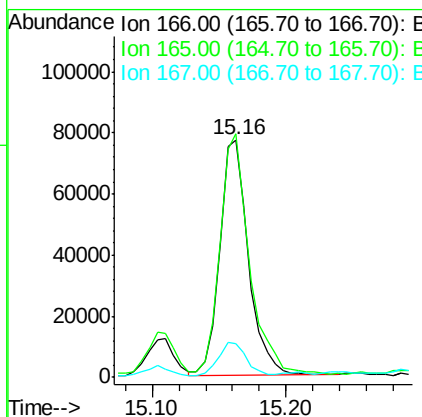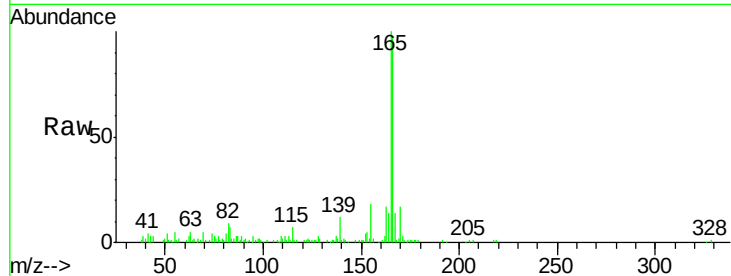

#69
Pentachlorophenol
Concen: 22.072 ng/ul
RT: 16.52 min Scan# 2317
Delta R.T. 0.01 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Tgt Ion	Ratio	Resp	Lower	Upper
266	100			
264	62.3	48.6	72.8	
268	63.6	50.6	76.0	

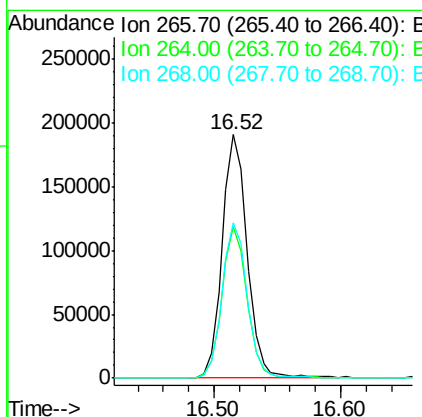

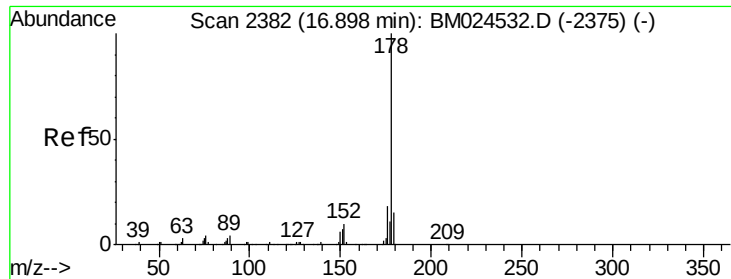

#70

Phenanthrene

Concen: 16.398 ng/ul

RT: 16.90 min Scan# 2382

Delta R.T. -0.00 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Instrument :

BNA_M

ClientSampleId :

GASG2MS

Tot Ion:178 Resp: 1295381

Ion Ratio Lower Upper

178 100

179 15.4 12.3 18.5





176 18.9 14.9 22.3

Manual Integrations

APPROVED

mohammad

1/21/2020 8:00:04 AM

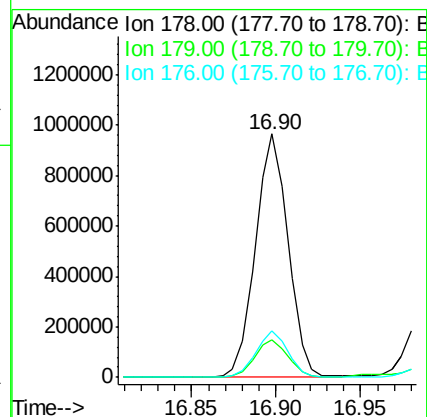

#72

Anthracene

Concen: 4.423 ng/ul

RT: 16.99 min Scan# 2397

Delta R.T. -0.00 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22




Tgt Ion:178 Resp: 356293


Ion Ratio Lower Upper

178 100

179 16.1 12.3 18.5

176 17.7 14.6 22.0

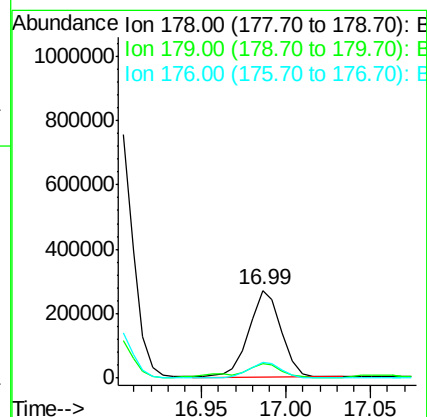

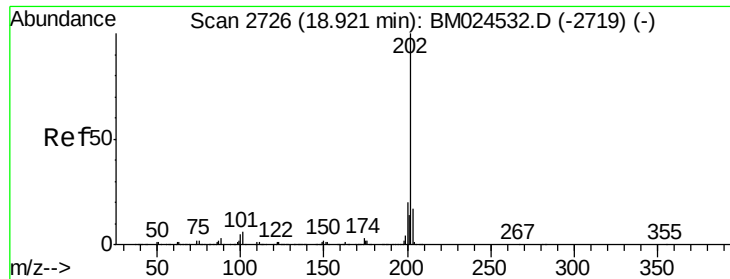





#77
 Fluoranthene
 Concen: 14.597 ng/ul
 RT: 18.93 min Scan# 2727
 Delta R.T. 0.01 min
 Lab File: BM024541.D
 Acq: 18 Jan 2020 18:22

Instrument :
 BNA_M
 ClientSampleId :
 GAS2MS

Tot Ion	Ratio	Resp	Lower	Upper
202	100	1409376		
101	6.8		5.4	8.2
100	5.5		4.3	6.5




Manual Integrations
 APPROVED


mohammad
 1/21/2020 8:00:04 AM

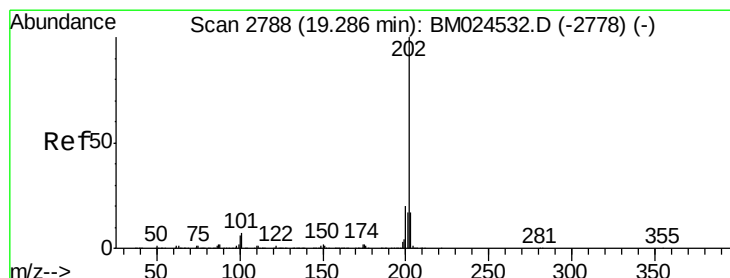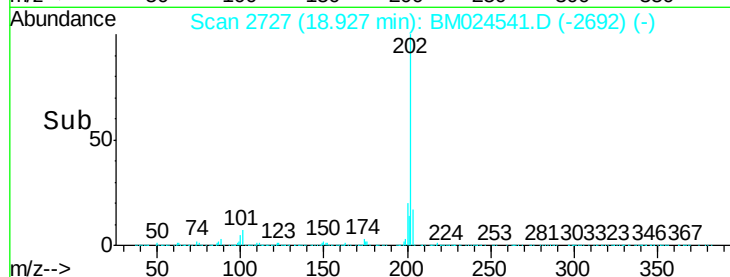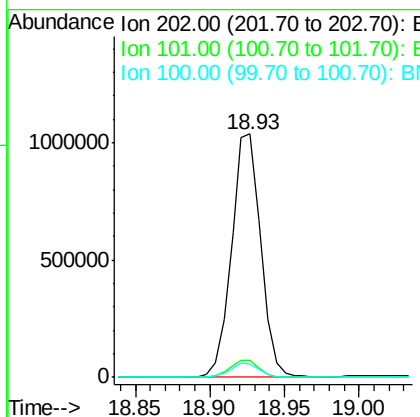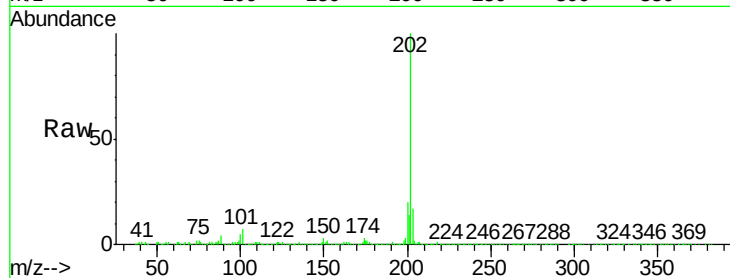

#80
 Pyrene
 Concen: 35.335 ng/ul
 RT: 19.29 min Scan# 2789
 Delta R.T. 0.01 min
 Lab File: BM024541.D
 Acq: 18 Jan 2020 18:22

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	3735982		
101	8.2		6.5	9.7
100	6.9		5.0	7.6

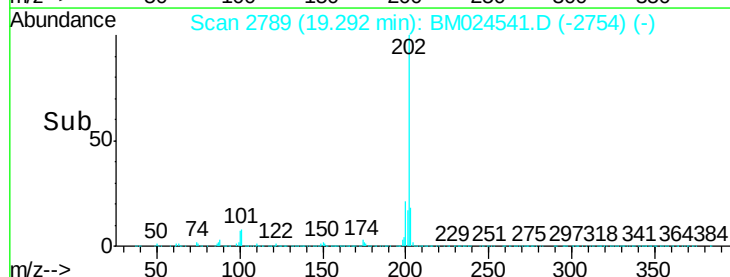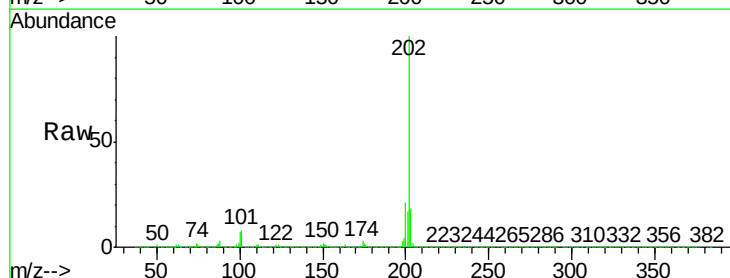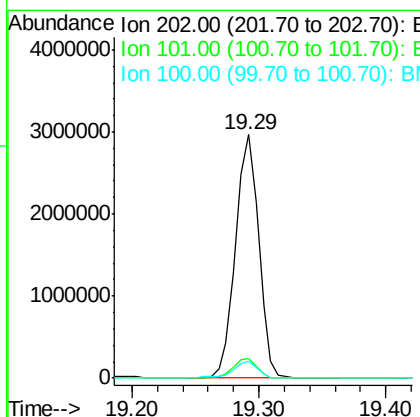

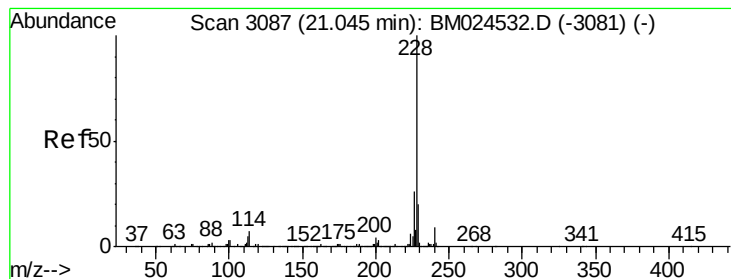

#83

Benzo(a)anthracene

Concen: 7.612 ng/ul

RT: 21.05 min Scan# 3088

Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Instrument :

BNA_M





ClientSampleId :

GASG2MS

Tot Ion:	228	Resp:	800833
Ion Ratio	Lower	Upper	
228	100		
229	20.4	15.9	23.9
226	33.6	21.1	31.7#

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

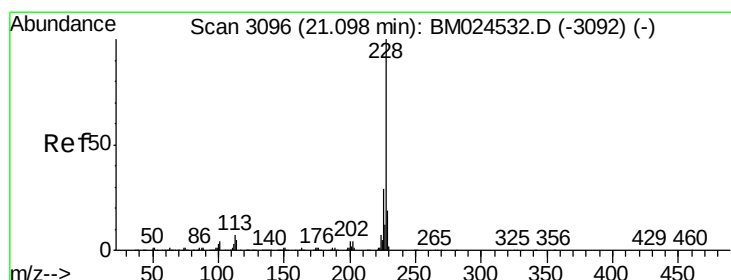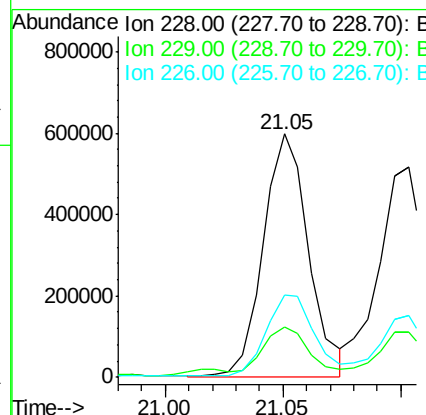

#85

Chrysene

Concen: 7.063 ng/ul




RT: 21.10 min Scan# 3097


Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Tgt Ion:	228	Resp:	716032
Ion Ratio	Lower	Upper	
228	100		
226	29.5	23.4	35.2
229	21.4	16.1	24.1

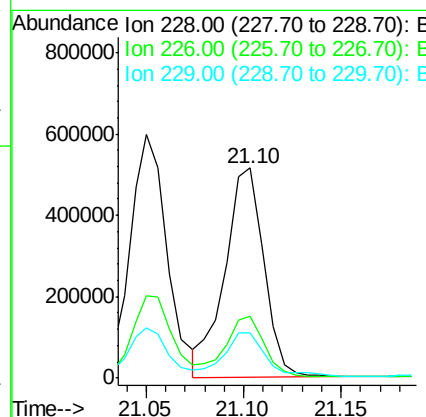



#88

Benzo(b)fluoranthene

Concen: 6.370 ng/ul

RT: 22.57 min Scan# 3346

Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Instrument :

BNA_M





ClientSampled :

GAS2MS

Tot Ion:	252	Resp:	691769
Ion Ratio	Lower	Upper	
252	100		
253	22.6	17.8	26.6
125	7.5	5.3	7.9

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

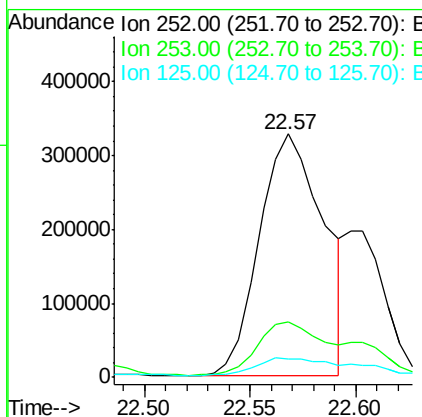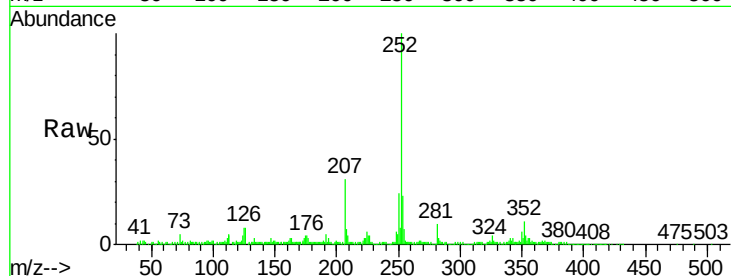

#89

Benzo(k)fluoranthene

Concen: 2.354 ng/ul m




RT: 22.60 min Scan# 3352


Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Tgt Ion:	252	Resp:	251203
Ion Ratio	Lower	Upper	
252	100		
253	23.8	17.1	25.7
125	8.4	5.2	7.8#

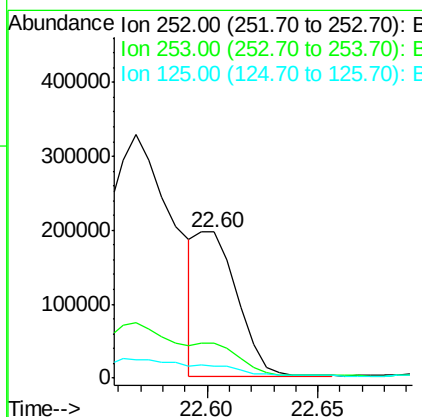

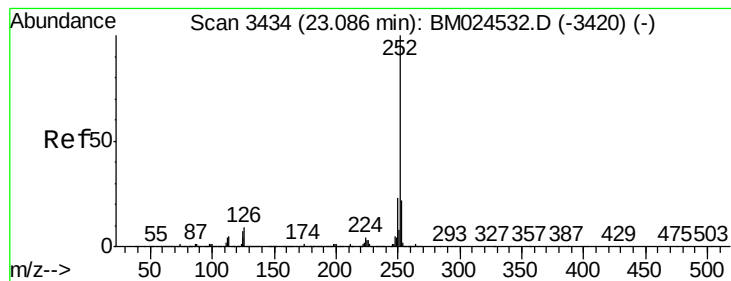

#91

Benzo(a)pyrene

Concen: 5.764 ng/ul

RT: 23.10 min Scan# 3436

Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Instrument :

BNA_M





ClientSampleId :

GAS2MS

Tot Ion	Ratio	Resp	Lower	Upper
252	100	543991		
253	22.2		17.5	26.3
125	7.6		5.7	8.5

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

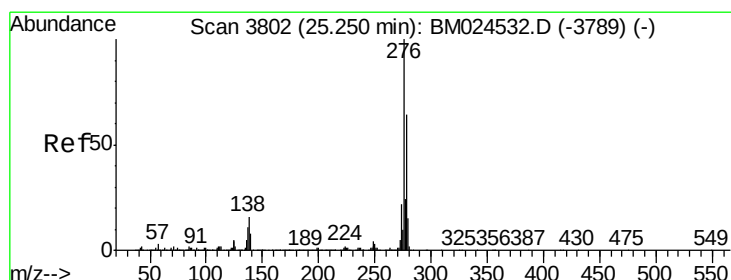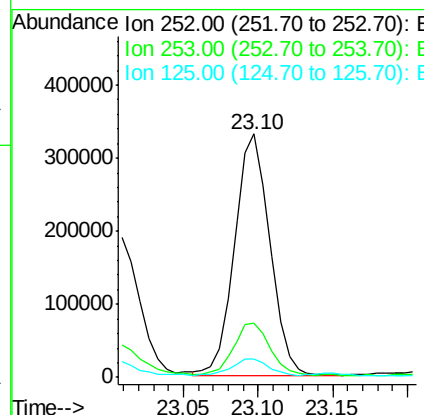

#92

Indeno(1,2,3-cd)pyrene

Concen: 2.849 ng/ul




RT: 25.26 min Scan# 3804


Delta R.T. 0.01 min

Lab File: BM024541.D

Acq: 18 Jan 2020 18:22

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	281346		
138	15.7		12.5	18.7
277	25.4		19.0	28.6

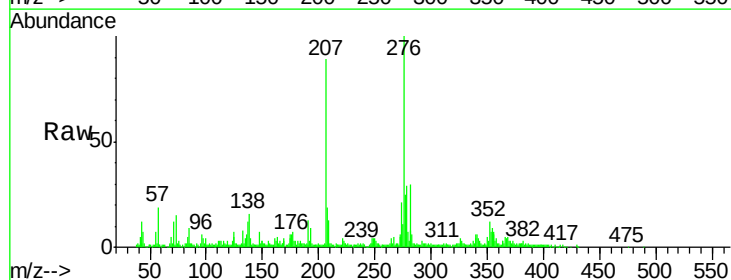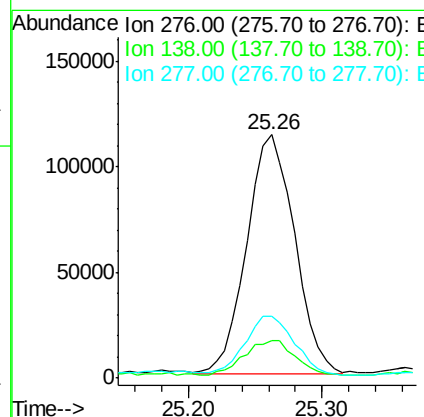

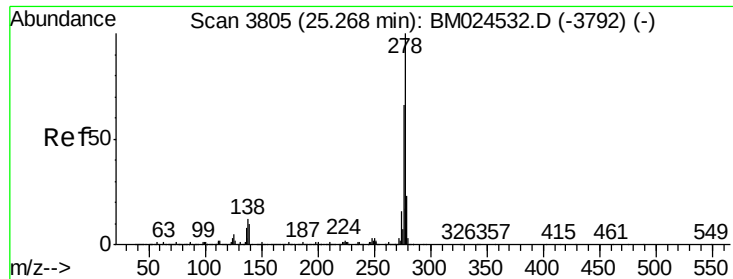





#93
Dibenzo(a,h)anthracene
Concen: 1.099 ng/ul
RT: 25.26 min Scan# 3804
Delta R.T. -0.01 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Instrument :
BNA_M
ClientSampleId :
GASG2MS

Tot Ion	Ratio	Lower	Upper
278	100		
139	14.6	8.7	13.1#
279	24.8	18.6	27.8

Manual Integrations
APPROVED

mohammad
1/21/2020 8:00:04 AM

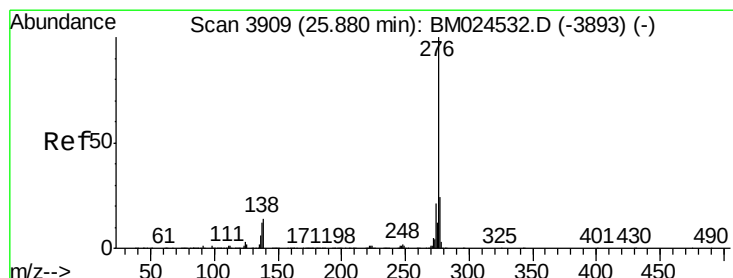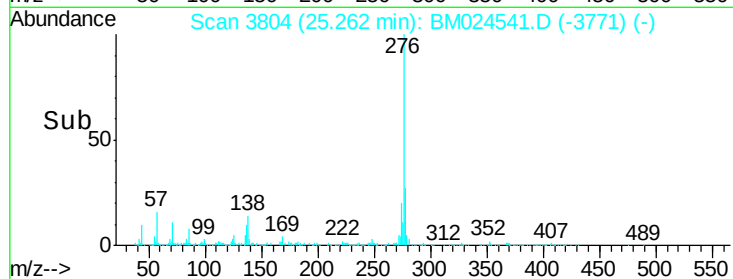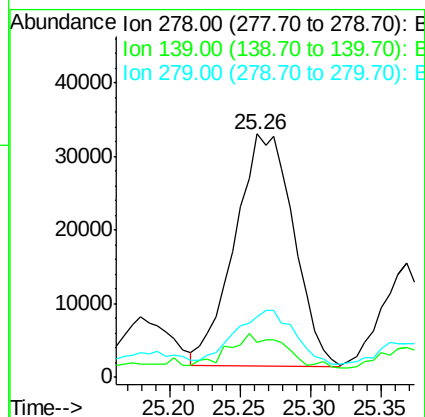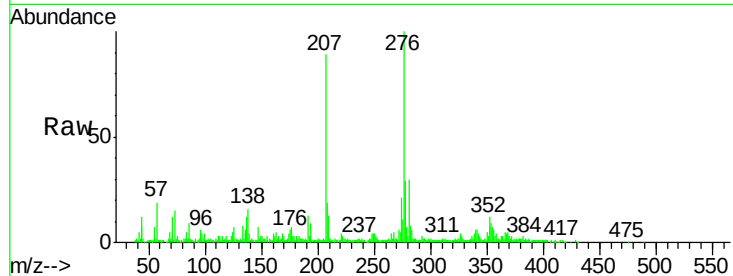

#94
Benzo(g,h,i)perylene
Concen: 2.520 ng/ul
RT: 25.89 min Scan# 3911
Delta R.T. 0.01 min
Lab File: BM024541.D
Acq: 18 Jan 2020 18:22

Tgt Ion	Ratio	Lower	Upper
276	100		
138	15.4	12.2	18.2
277	23.0	18.8	28.2

