

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011722\
 Data File : BM033752.D
 Acq On : 17 Jan 2022 16:50
 Operator : CG/JU
 Sample : PB142053BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB142053BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.502	378	385	397	rBV	3096003	4432714	39.67%	9.420%
2	7.113	651	659	672	rBV	2871820	4598425	41.16%	9.773%
3	7.954	795	802	811	rBV	580702	911112	8.15%	1.936%
4	9.119	990	1000	1009	rBV	1853229	3027217	27.09%	6.434%
5	10.772	1273	1281	1289	rBV	758403	1299984	11.63%	2.763%
6	13.225	1691	1698	1711	rBV	4913946	7222166	64.64%	15.349%
7	14.595	1922	1931	1942	rBV	1214269	1846913	16.53%	3.925%
8	16.071	2175	2182	2196	rBV	3999308	5713803	51.14%	12.143%
9	17.324	2389	2395	2408	rBV	1538416	2297005	20.56%	4.882%
10	19.942	2834	2840	2850	rBV	8867838	11173097	100.00%	23.745%
11	21.495	3099	3104	3110	rBV	1864355	2340154	20.94%	4.973%
12	23.906	3507	3514	3523	rVB2	1101815	2191372	19.61%	4.657%




Sum of corrected areas: 47053962

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011722\
Data File : BM033752.D
Acq On : 17 Jan 2022 16:50
Operator : CG/JU
Sample : PB142053BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142053BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

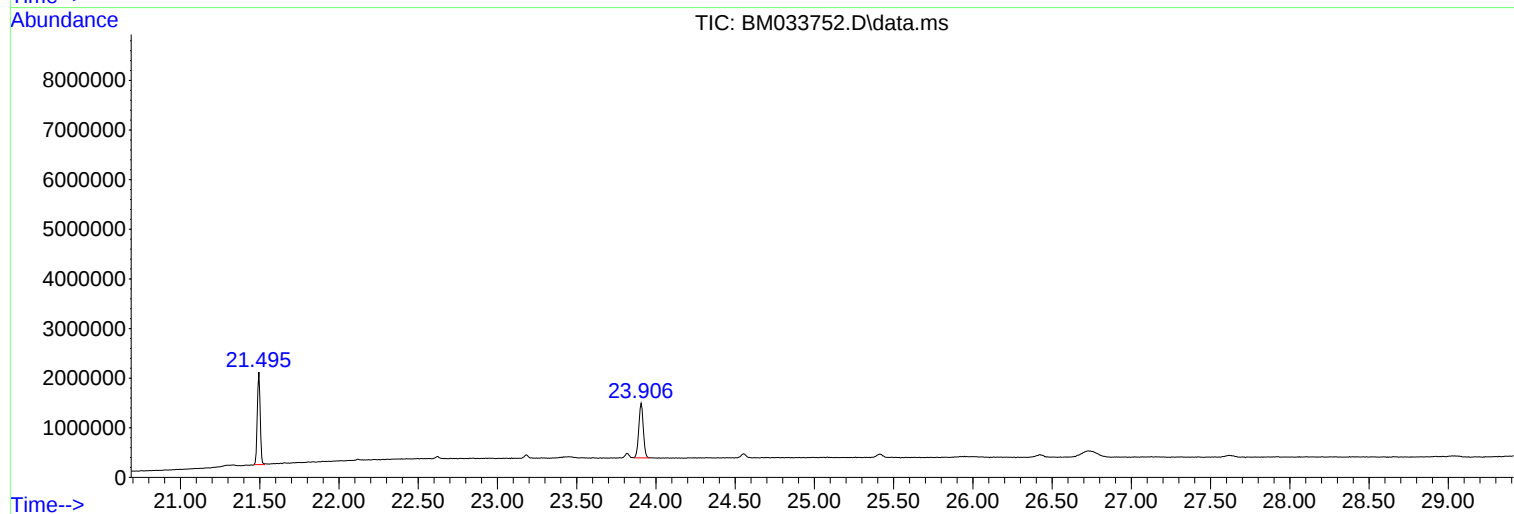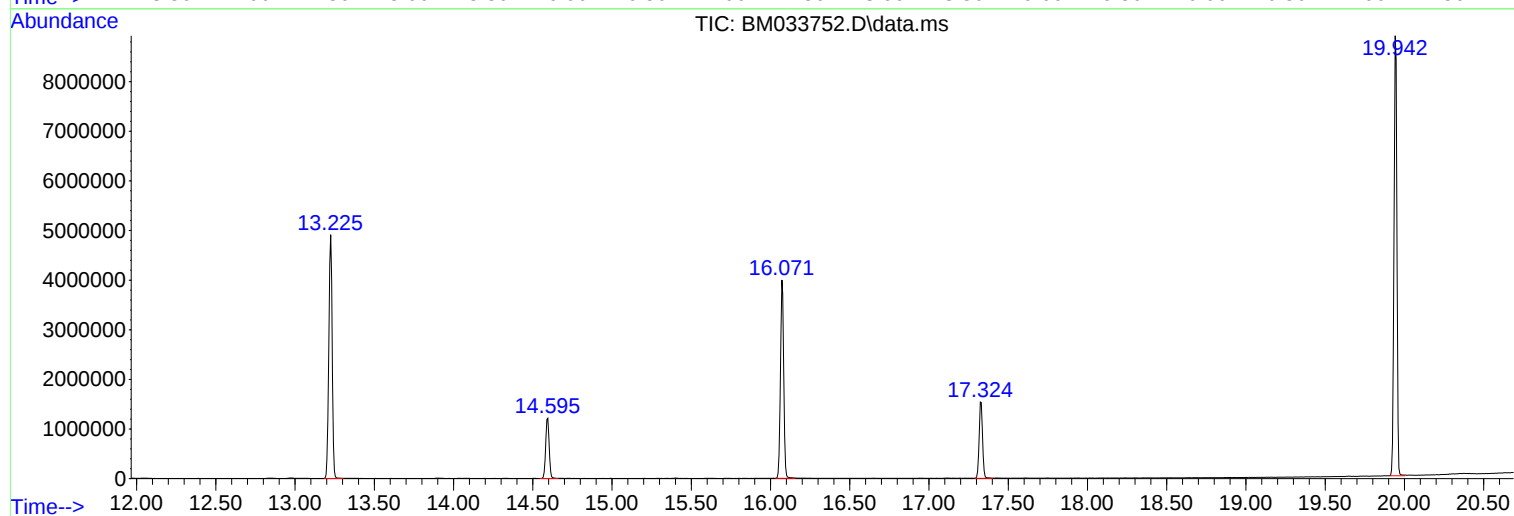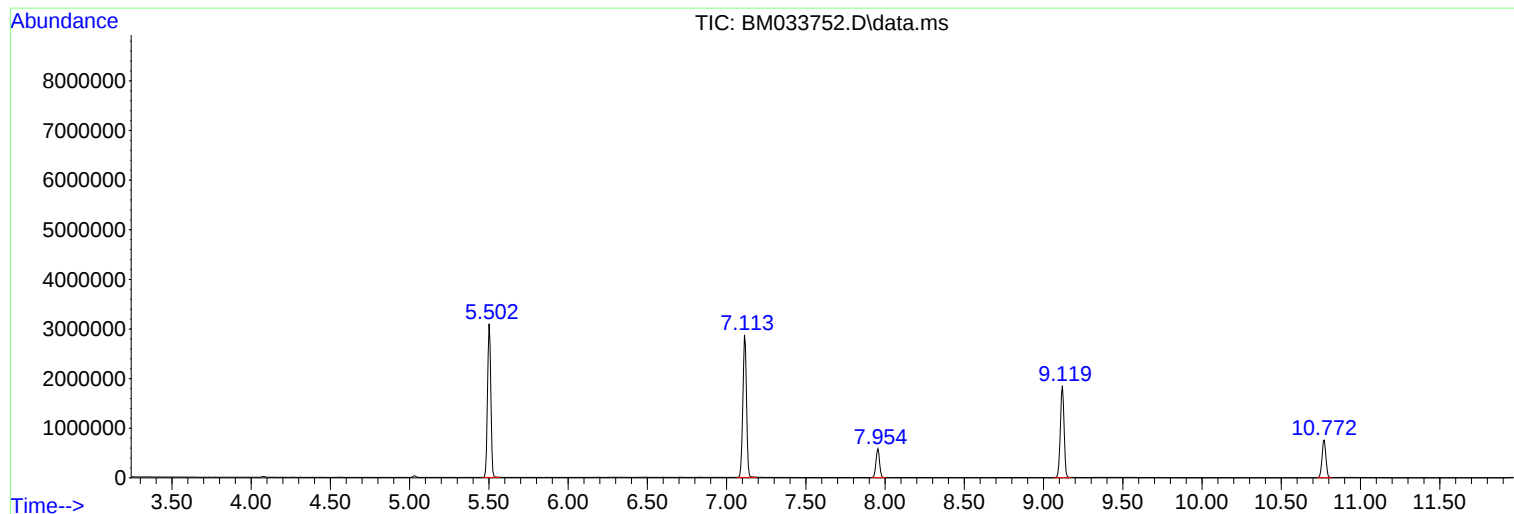

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011722\
Data File : BM033752.D
Acq On : 17 Jan 2022 16:50
Operator : CG/JU
Sample : PB142053BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142053BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011722\
Data File : BM033752.D
Acq On : 17 Jan 2022 16:50
Operator : CG/JU
Sample : PB142053BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142053BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------