

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011722\  
 Data File : BM033754.D  
 Acq On : 17 Jan 2022 18:02  
 Operator : CG/JU  
 Sample : PB142051BL  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB142051BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM011722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033754.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.501       | 378           | 385         | 394          | rBV      | 2104547        | 2959871       | 26.29%          | 7.051%        |
| 2         | 7.113       | 651           | 659         | 669          | rBV      | 1967529        | 3080212       | 27.36%          | 7.338%        |
| 3         | 7.954       | 792           | 802         | 810          | rVB      | 573773         | 884414        | 7.85%           | 2.107%        |
| 4         | 9.119       | 992           | 1000        | 1012         | rBV      | 1799803        | 2943763       | 26.14%          | 7.013%        |
| 5         | 10.766      | 1273          | 1280        | 1293         | rBV      | 723062         | 1256650       | 11.16%          | 2.994%        |
| 6         | 13.224      | 1690          | 1698        | 1712         | rBV      | 4741710        | 7018781       | 62.33%          | 16.720%       |
| 7         | 14.589      | 1924          | 1930        | 1942         | rBV      | 1229855        | 1781219       | 15.82%          | 4.243%        |
| 8         | 16.071      | 2175          | 2182        | 2200         | rBV      | 2732468        | 3776461       | 33.54%          | 8.996%        |
| 9         | 17.324      | 2389          | 2395        | 2409         | rBV      | 1552444        | 2224035       | 19.75%          | 5.298%        |
| 10        | 19.942      | 2834          | 2840        | 2852         | rBV      | 9513820        | 11259779      | 100.00%         | 26.823%       |
| 11        | 21.489      | 3098          | 3103        | 3112         | rBV      | 1875836        | 2402008       | 21.33%          | 5.722%        |
| 12        | 23.900      | 3506          | 3513        | 3526         | rVB2     | 1156443        | 2390163       | 21.23%          | 5.694%        |




Sum of corrected areas: 41977356

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011722\  
Data File : BM033754.D  
Acq On : 17 Jan 2022 18:02  
Operator : CG/JU  
Sample : PB142051BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB142051BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM011722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

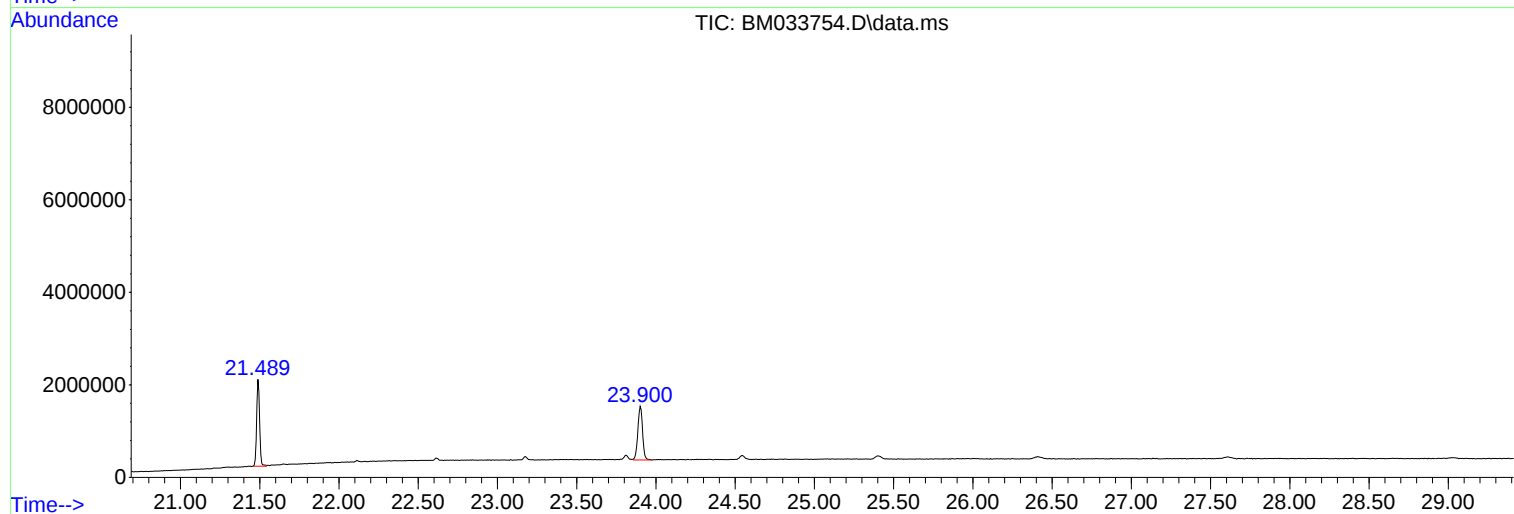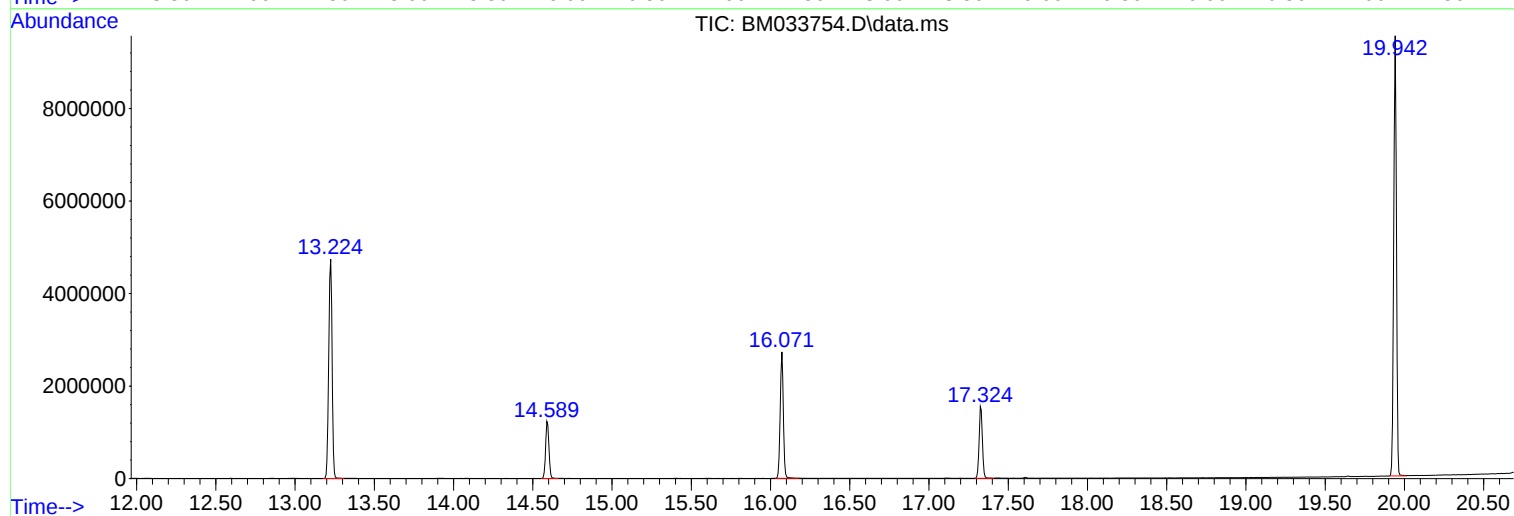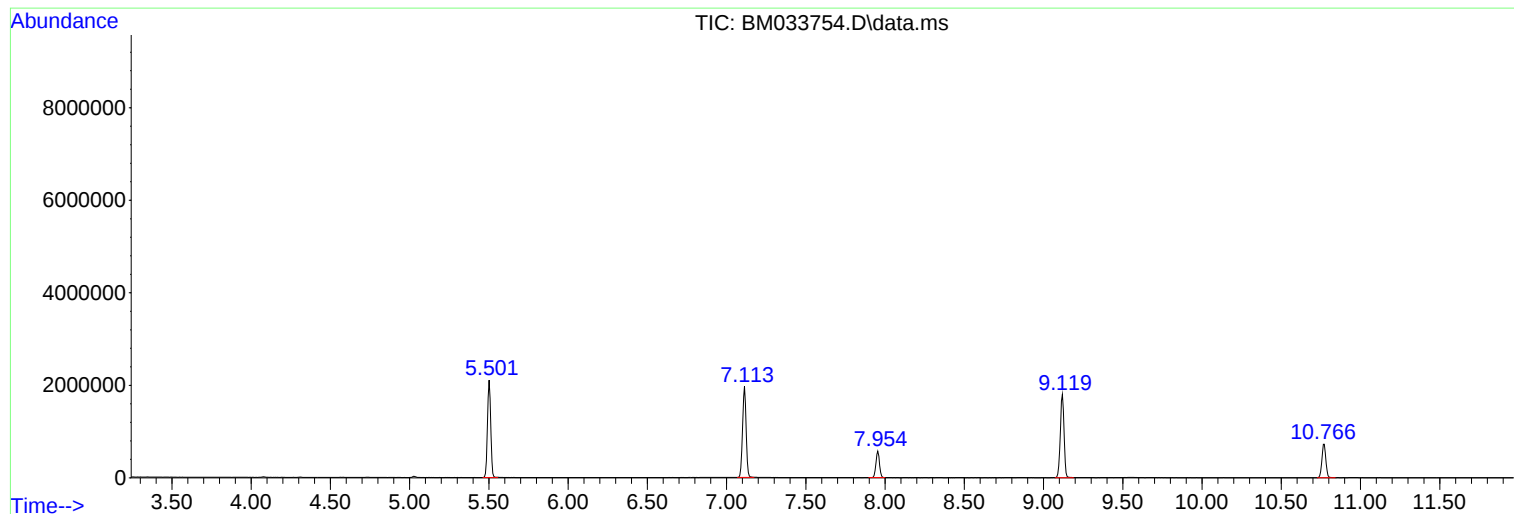

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011722\  
Data File : BM033754.D  
Acq On : 17 Jan 2022 18:02  
Operator : CG/JU  
Sample : PB142051BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB142051BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM011722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011722\  
Data File : BM033754.D  
Acq On : 17 Jan 2022 18:02  
Operator : CG/JU  
Sample : PB142051BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB142051BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM011722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|