




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043867.D
Acq On : 17 Jan 2024 15:11
Operator : MA/JU
Sample : P1142-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B64

Manual IntegrationsAPPROVED

Quant Time: Jan 17 15:45:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 10 01:07:47 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/18/2024
Supervised By :mohammad ahmed 01/19/2024

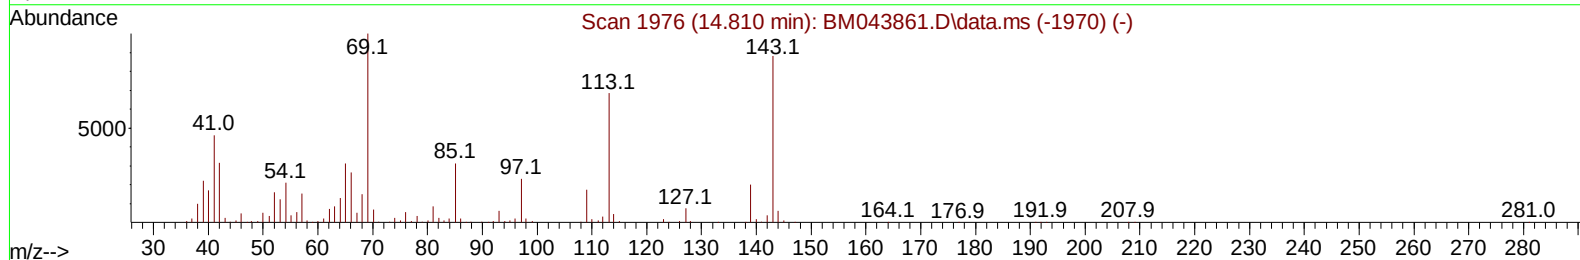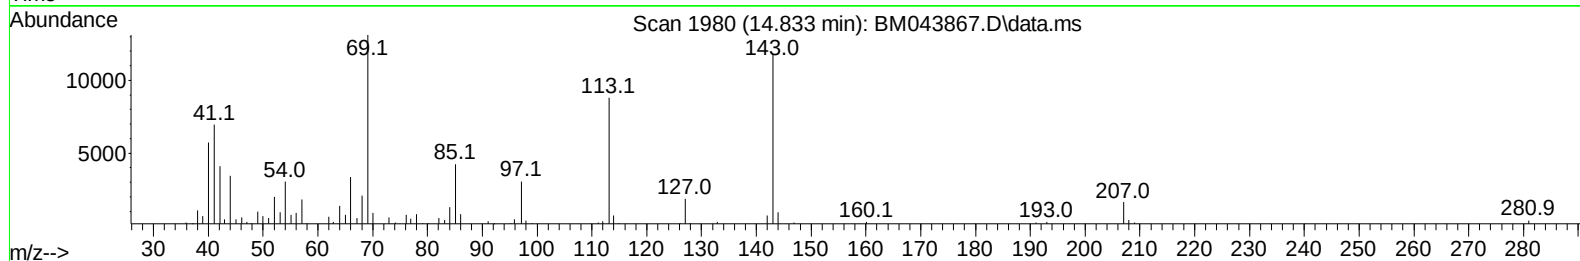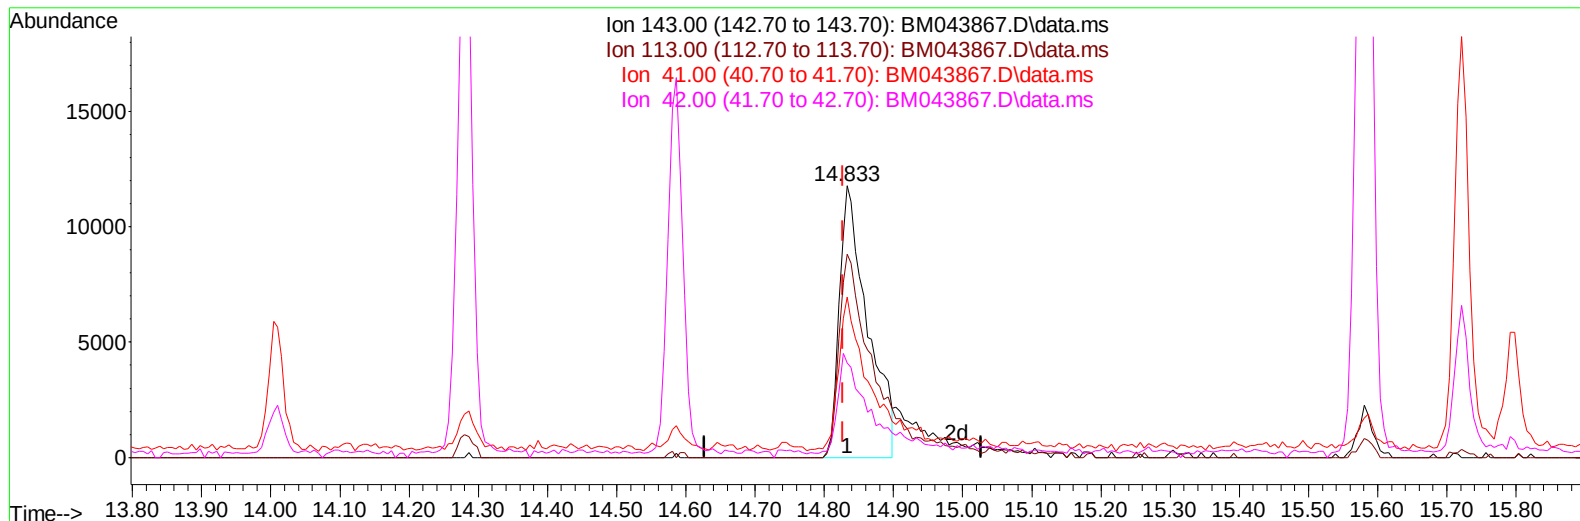

TIC: BM043867.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.833min (+ 0.006) 3.36 ng/u1

response 33225

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.20	74.91
41.00	44.00	59.01#
42.00	30.80	34.74




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043867.D
 Acq On : 17 Jan 2024 15:11
 Operator : MA/JU
 Sample : P1142-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B64

Manual IntegrationsAPPROVED

Quant Time: Jan 17 15:45:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 10 01:07:47 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/18/2024
 Supervised By :mohammad ahmed 01/19/2024

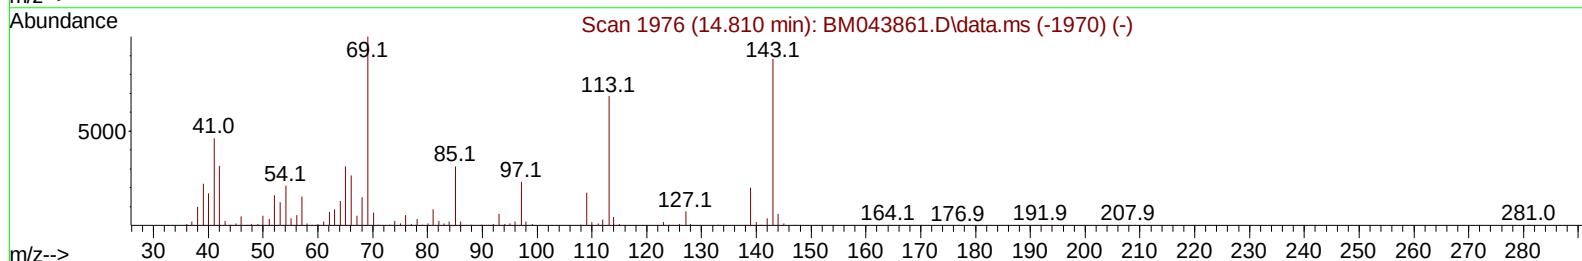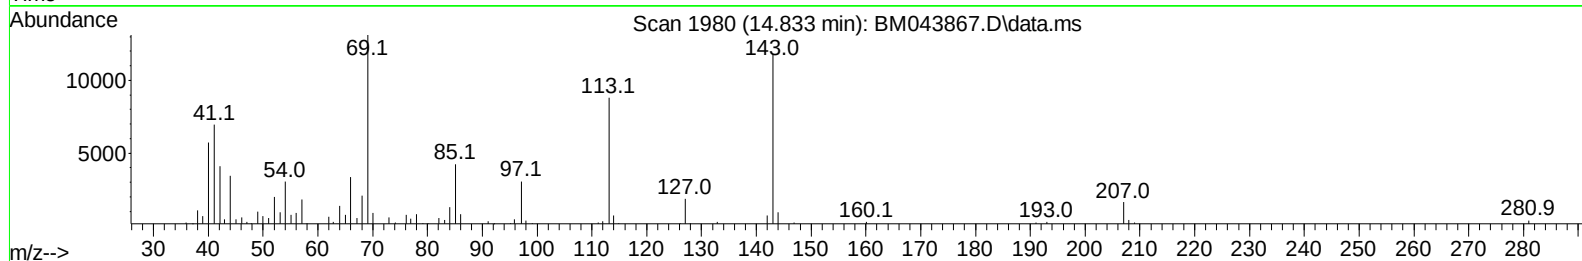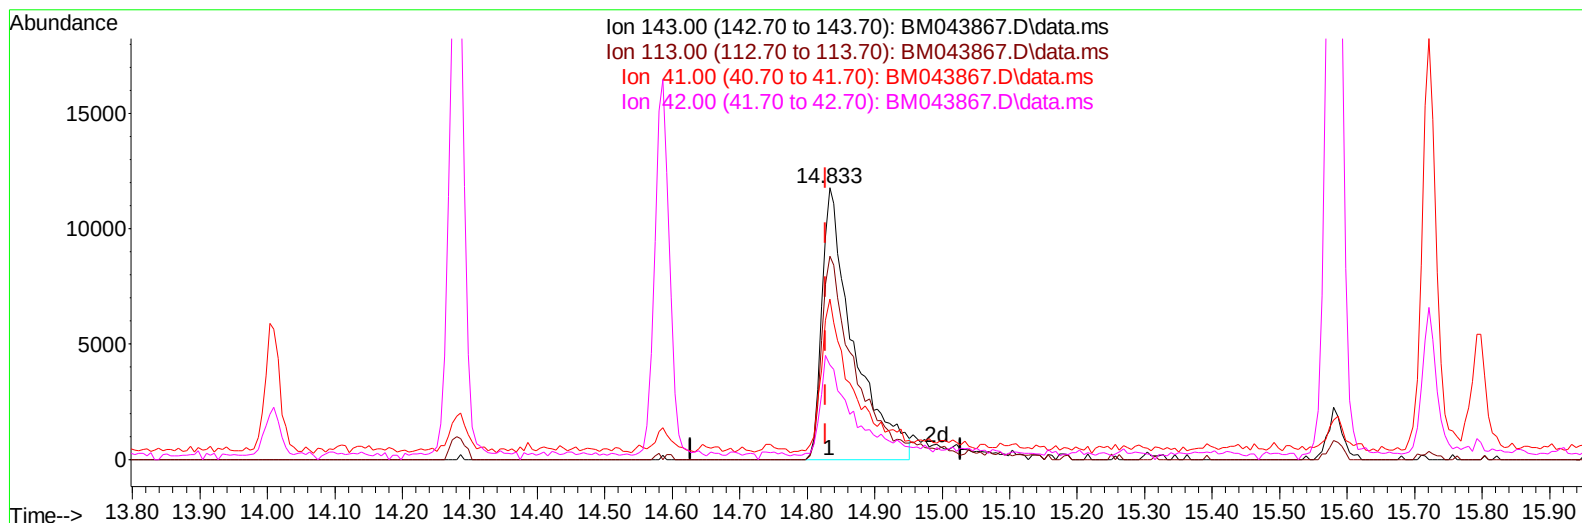

TIC: BM043867.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.833min (+ 0.006) 3.84 ng/ul m

response 38008

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.20	74.91
41.00	44.00	59.01#
42.00	30.80	34.74

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043867.D
 Acq On : 17 Jan 2024 15:11
 Operator : MA/JU
 Sample : P1142-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B64

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/18/2024
 Supervised By :mohammad ahmed 01/19/2024

Quant Time: Jan 18 00:10:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 10 01:07:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	194348	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.751	136	906254	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	603576	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1331644	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	1206103	20.000	ng/ul	0.00
88) Perylene-d12	23.950	264	1357235	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	19257	3.826	ng/uL	0.00
4) Pyridine-d5	3.787	84	90899	5.862	ng/ul	0.00
7) Phenol-d5	7.116	99	106945	5.438	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	453034	36.963	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.469	132	373227	26.086	ng/ul	-0.01
15) 4-Methylphenol-d8	8.663	113	225194	14.374	ng/ul	-0.01
21) Nitrobenzene-d5	9.122	128	276031	36.343	ng/ul	0.00
24) 2-Nitrophenol-d4	9.839	143	282592	33.042	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	464610	30.336	ng/ul	0.00
31) 4-Chloroaniline-d4	10.904	131	680538	28.055	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	1908605	37.752	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	2223158	38.605	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.833	143	38008m	3.844	ng/ul	0.00
60) Fluorene-d10	15.580	176	1730383	40.671	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.721	200	214855	22.852	ng/ul	0.00
73) Anthracene-d10	17.439	188	2749144	40.567	ng/ul	0.00
81) Pyrene-d10	19.733	212	3179319	42.678	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.791	264	3180603	42.453	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043867.D
Acq On : 17 Jan 2024 15:11
Operator : MA/JU
Sample : P1142-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B64

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/18/2024
Supervised By :mohammad ahmed 01/19/2024

Quant Time: Jan 18 00:10:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 10 01:07:47 2024
Response via : Initial Calibration

