

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043863.D
 Acq On : 17 Jan 2024 12:46
 Operator : MA/JU
 Sample : P1130-15
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AZ5

Quant Time: Jan 17 14:28:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 10 01:07:47 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	242028	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.751	136	1141192	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	775833	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1631161	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	1530628	20.000	ng/ul	0.00
88) Perylene-d12	23.950	264	1642329	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	25063	3.998	ng/uL	0.00
4) Pyridine-d5	3.781	84	198599	10.285	ng/ul	0.00
7) Phenol-d5	7.110	99	142703	5.826	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.281	67	493547	32.335	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.469	132	418697	23.499	ng/ul	-0.01
15) 4-Methylphenol-d8	8.663	113	289681	14.847	ng/ul	-0.01
21) Nitrobenzene-d5	9.122	128	307319	32.133	ng/ul	0.00
24) 2-Nitrophenol-d4	9.839	143	306011	28.414	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	565337	29.313	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.904	131	572902	18.756	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	2341945	36.038	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	2644755	35.730	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.833	143	80988	6.372	ng/ul	0.00
60) Fluorene-d10	15.580	176	2122636	38.813	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.721	200	318449	27.651	ng/ul	0.00
73) Anthracene-d10	17.439	188	3403447	41.001	ng/ul	0.00
81) Pyrene-d10	19.733	212	4040814	42.742	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.797	264	3858364	42.559	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.387	88	9543	1.451	ng/uL#	77
78) Di-n-butylphthalate	18.315	149	527732	4.112	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043863.D
Acq On : 17 Jan 2024 12:46
Operator : MA/JU
Sample : P1130-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AZ5

Quant Time: Jan 17 14:28:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 10 01:07:47 2024
Response via : Initial Calibration




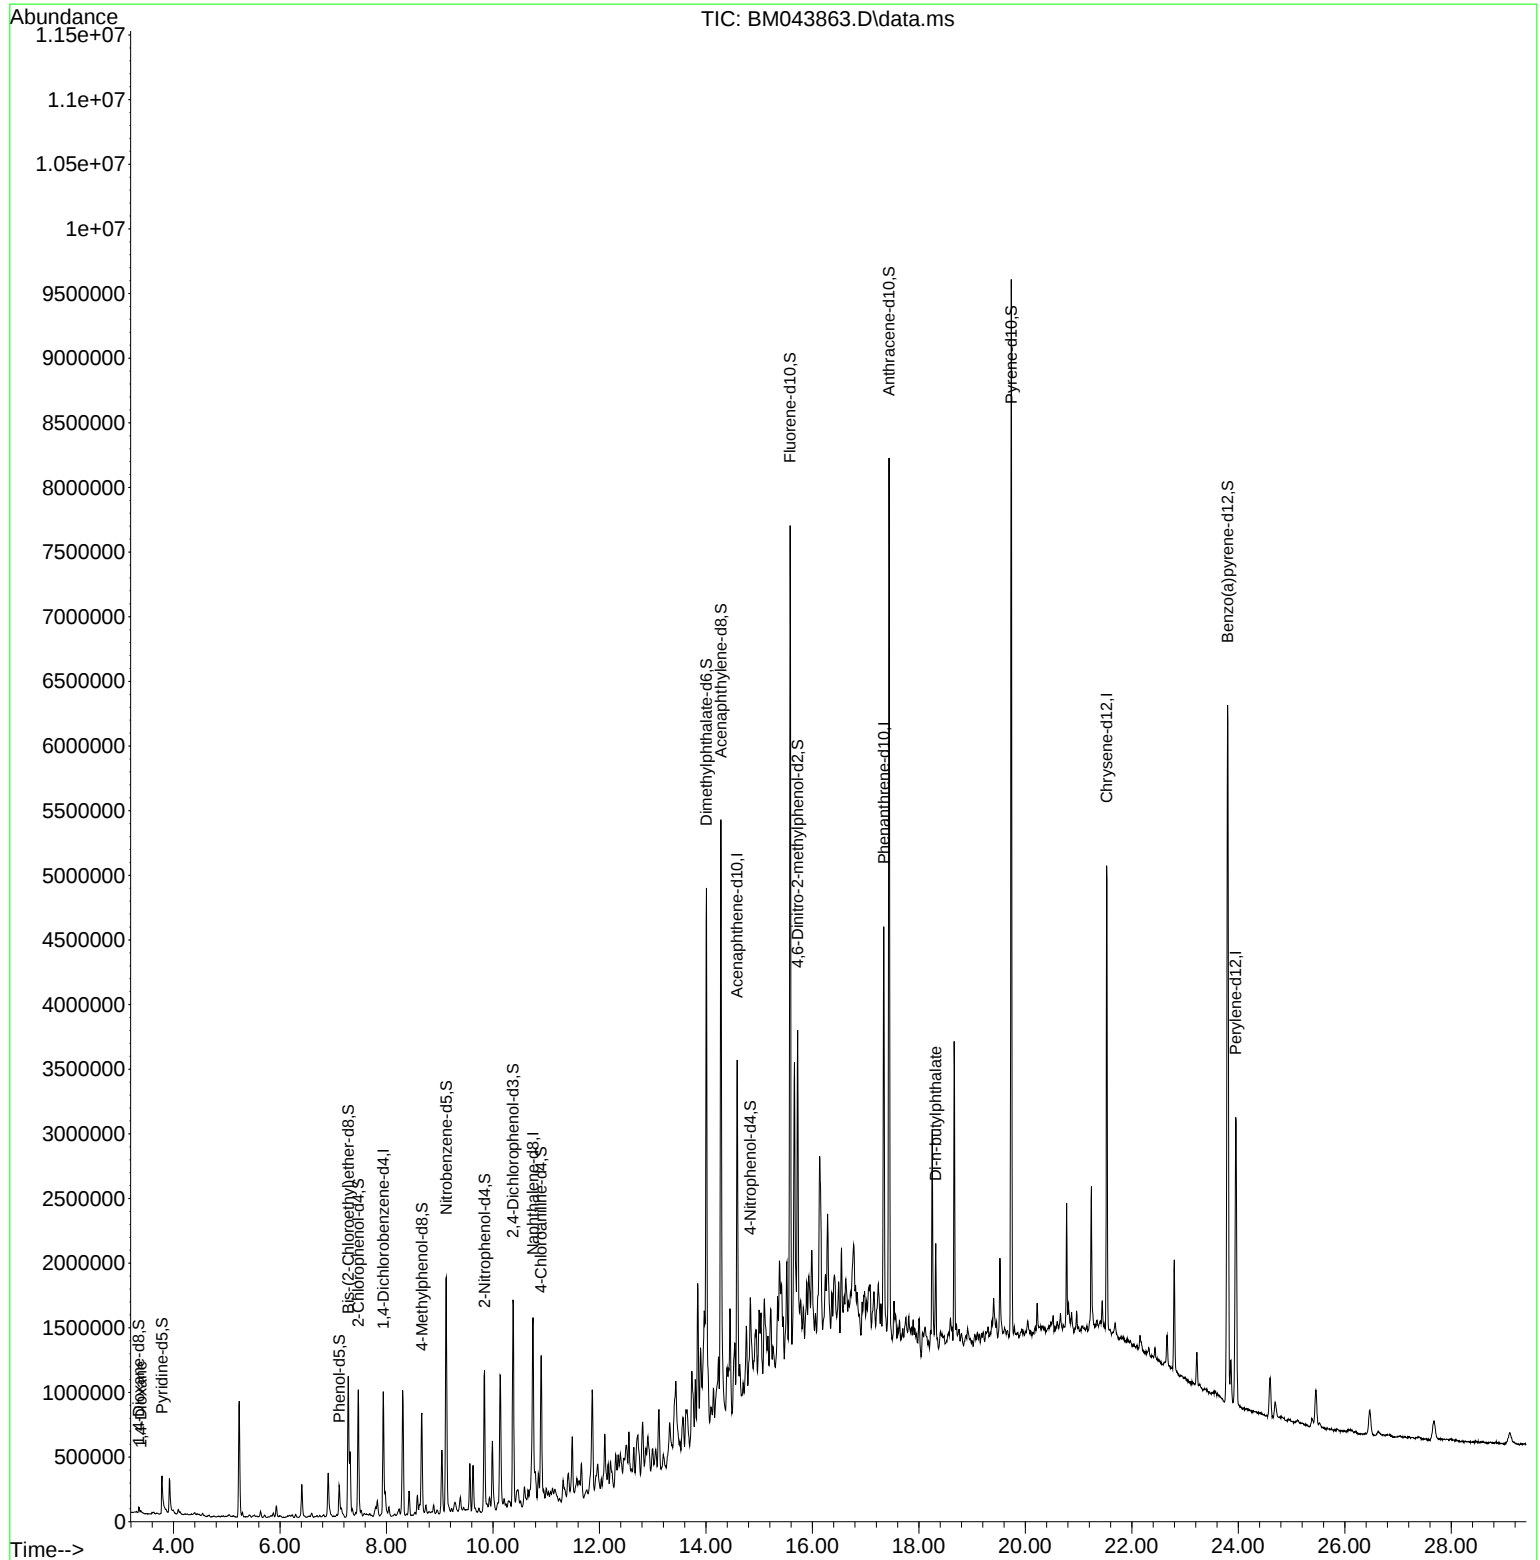


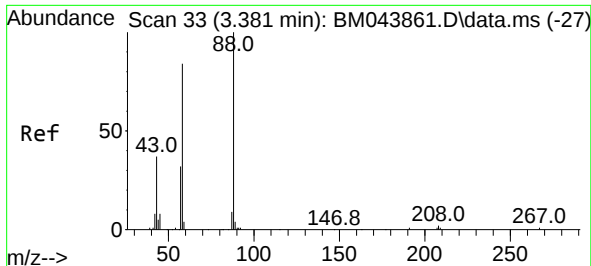

#2
1,4-Dioxane
Concen: 1.451 ng/uL
RT: 3.387 min Scan# 34
Delta R.T. -0.006 min
Lab File: BM043863.D
Acq: 17 Jan 2024 12:46

Instrument :
BNA_M
ClientSampleId :
C0AZ5

Tgt Ion: 88 Resp: 9543
Ion Ratio Lower Upper
88 100
43 60.5 27.2 40.8#
58 66.7 62.6 93.8

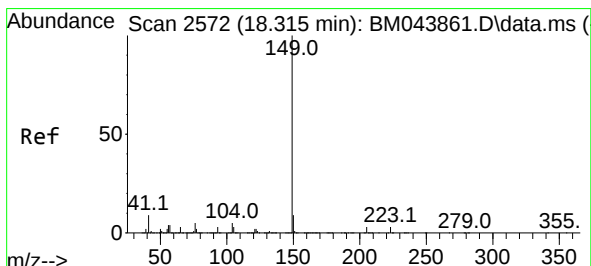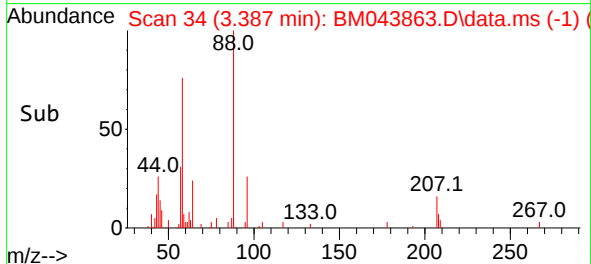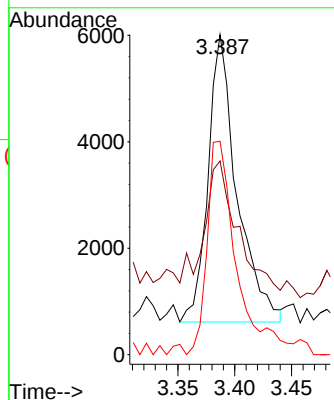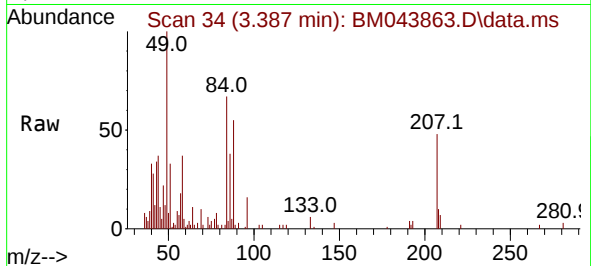

#78
Di-n-butylphthalate
Concen: 4.112 ng/uL
RT: 18.315 min Scan# 2572
Delta R.T. -0.006 min
Lab File: BM043863.D
Acq: 17 Jan 2024 12:46

Tgt Ion: 149 Resp: 527732
Ion Ratio Lower Upper
149 100
150 9.8 7.3 10.9
104 6.1 3.8 5.8#

