

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043862.D
 Acq On : 17 Jan 2024 12:10
 Operator : MA/JU
 Sample : PB158463BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK463

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	33	rBV	64755	90741	1.20%	0.115%
2	3.775	96	100	128	rBV	830796	1658162	21.93%	2.107%
3	4.087	151	153	161	rVB3	14289	20935	0.28%	0.027%
4	7.110	660	667	680	rBV	1139967	1978446	26.16%	2.513%
5	7.281	689	696	707	rBV	976279	1594322	21.08%	2.025%
6	7.469	721	728	737	rBV	1150698	1922429	25.42%	2.442%
7	7.939	800	808	823	rBV	951703	1527927	20.20%	1.941%
8	8.657	923	930	949	rBV	1400584	2426098	32.08%	3.082%
9	9.116	1002	1008	1022	rBV	1154545	2021486	26.73%	2.568%
10	9.839	1124	1131	1145	rBV	1000365	1714795	22.68%	2.179%
11	10.375	1215	1222	1248	rBV	1276592	2432667	32.17%	3.090%
12	10.751	1278	1286	1300	rVB	1411144	2368856	31.32%	3.009%
13	10.904	1305	1312	1333	rBV	1224409	2601092	34.40%	3.304%
14	12.369	1554	1561	1567	rVB	18221	35515	0.47%	0.045%
15	13.486	1745	1751	1758	rBV	24386	41573	0.55%	0.053%
16	13.568	1762	1765	1772	rVB9	5742	8316	0.11%	0.011%
17	13.963	1827	1832	1834	rBV5	5535	9794	0.13%	0.012%
18	14.010	1834	1840	1852	rVV	2842515	4007272	52.99%	5.091%
19	14.280	1879	1886	1898	rBV	3156390	4788376	63.32%	6.083%
20	14.586	1931	1938	1950	rBV	2293334	3339728	44.16%	4.243%
21	14.815	1970	1977	1998	rBV	990071	1939563	25.65%	2.464%
22	15.580	2101	2107	2119	rBV	4042972	6030549	79.75%	7.661%
23	15.721	2125	2131	2145	rBV	1280081	1931213	25.54%	2.453%
24	15.821	2146	2148	2156	rVB2	20869	34081	0.45%	0.043%
25	16.368	2236	2241	2245	rBV6	12299	18020	0.24%	0.023%
26	17.015	2346	2351	2358	rBV7	7301	9347	0.12%	0.012%
27	17.133	2367	2371	2374	rBV3	5990	9718	0.13%	0.012%
28	17.339	2399	2406	2417	rBV	2812498	3972967	52.54%	5.047%
29	17.439	2417	2423	2435	rBV	4490506	6423436	84.94%	8.160%
30	18.021	2518	2522	2527	rBV7	4647	8773	0.12%	0.011%
31	18.251	2557	2561	2563	rBV5	6820	10303	0.14%	0.013%
32	19.297	2735	2739	2745	rBV3	47644	73076	0.97%	0.093%
33	19.374	2747	2752	2756	rBV	39415	55772	0.74%	0.071%
34	19.668	2799	2802	2805	rBV5	8805	12297	0.16%	0.016%
35	19.733	2807	2813	2828	rBV	5592213	7456425	98.60%	9.473%
36	21.533	3113	3119	3130	rBV	3010758	4191556	55.43%	5.325%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043862.D
Acq On : 17 Jan 2024 12:10
Operator : MA/JU
Sample : PB158463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK463

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Title : SVOA CALIBRATION

37	23.797	3496	3504	3511	rBV2	3977947	7562221	100.00%	9.607%
38	23.956	3523	3531	3543	rVB	2097044	4386630	58.01%	5.573%




Sum of corrected areas: 78714477

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043862.D
Acq On : 17 Jan 2024 12:10
Operator : MA/JU
Sample : PB158463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK463

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

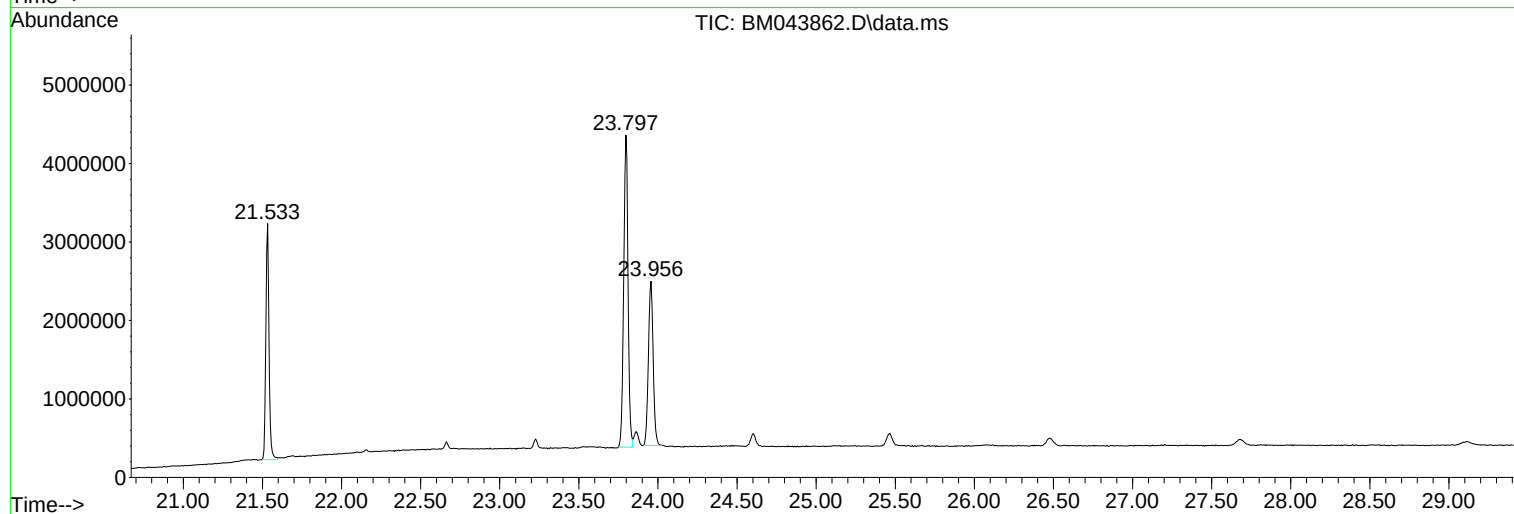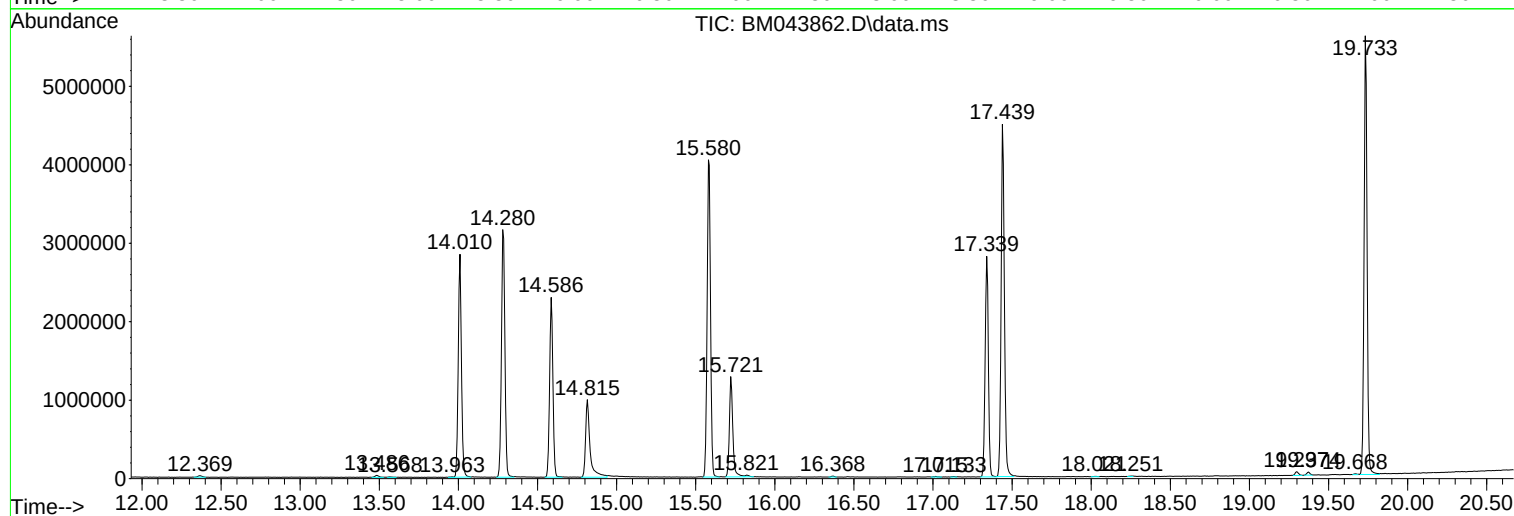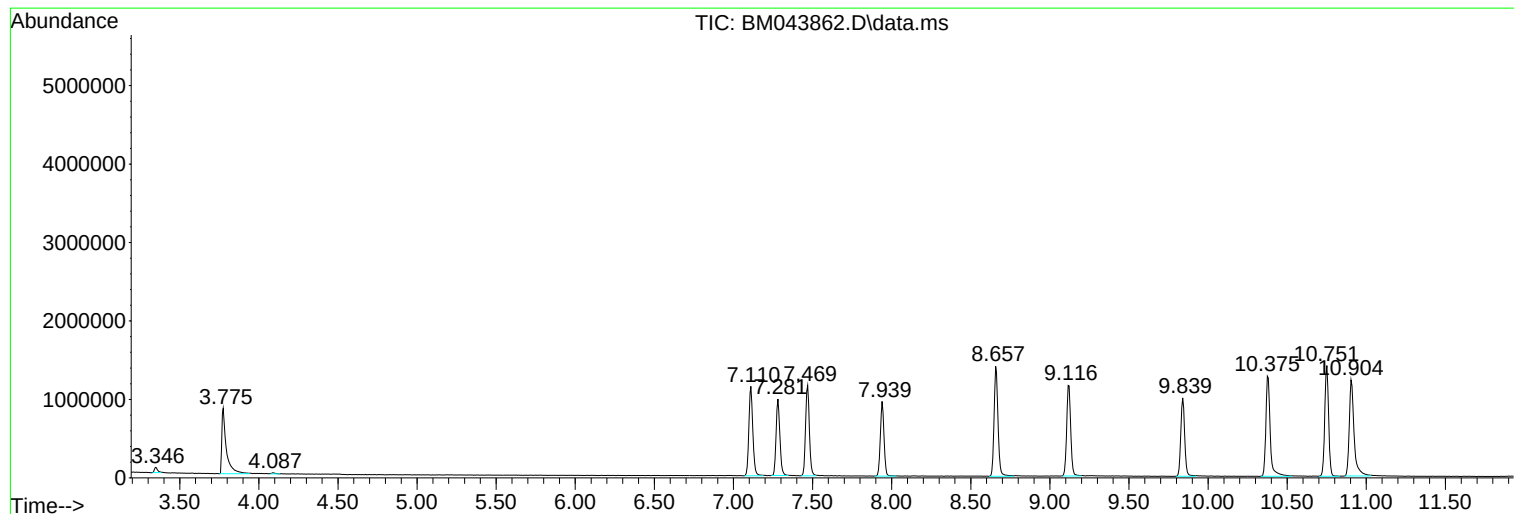

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043862.D
Acq On : 17 Jan 2024 12:10
Operator : MA/JU
Sample : PB158463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK463

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043862.D
Acq On : 17 Jan 2024 12:10
Operator : MA/JU
Sample : PB158463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK463

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------