

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043867.D
 Acq On : 17 Jan 2024 15:11
 Operator : MA/JU
 Sample : P1142-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	39	rVB	36770	64049	0.74%	0.087%
2	3.793	99	103	114	rBV	117990	266299	3.06%	0.363%
3	4.093	151	154	161	rVB2	15332	23800	0.27%	0.032%
4	7.116	661	668	677	rBV	173331	330413	3.80%	0.450%
5	7.281	690	696	714	rBV	955505	1588888	18.25%	2.163%
6	7.469	721	728	739	rBV	838216	1410975	16.21%	1.921%
7	7.940	801	808	818	rBV	735046	1209231	13.89%	1.646%
8	8.663	922	931	941	rBV	599770	1052082	12.09%	1.432%
9	8.787	948	952	958	rVB	29055	45455	0.52%	0.062%
10	9.122	1000	1009	1022	rBV	1190406	2075426	23.84%	2.825%
11	9.475	1065	1069	1079	rVB2	22395	38939	0.45%	0.053%
12	9.839	1122	1131	1141	rBV	948948	1628262	18.70%	2.217%
13	10.381	1214	1223	1240	rBV	1177249	2267872	26.05%	3.087%
14	10.751	1278	1286	1298	rBV	1117497	1912827	21.97%	2.604%
15	10.904	1304	1312	1336	rBV	1097803	2340517	26.89%	3.186%
16	11.322	1378	1383	1389	rBV2	10457	22746	0.26%	0.031%
17	11.380	1389	1393	1402	rVB4	9453	23600	0.27%	0.032%
18	11.769	1455	1459	1469	rVB7	8457	18303	0.21%	0.025%
19	11.975	1487	1494	1501	rVB	23191	35435	0.41%	0.048%
20	12.357	1554	1559	1568	rVB2	20032	39663	0.46%	0.054%
21	12.486	1577	1581	1588	rVB9	9707	18482	0.21%	0.025%
22	12.704	1613	1618	1621	rBV7	5174	9580	0.11%	0.013%
23	12.857	1639	1644	1646	rBV5	5711	8968	0.10%	0.012%
24	13.045	1667	1676	1686	rBV2	21216	58477	0.67%	0.080%
25	13.480	1745	1750	1758	rVV	37410	60175	0.69%	0.082%
26	13.604	1767	1771	1776	rVB4	13611	21866	0.25%	0.030%
27	14.010	1833	1840	1853	rVB	2921044	4215555	48.42%	5.739%
28	14.280	1879	1886	1902	rBV	3603083	5190800	59.63%	7.067%
29	14.586	1931	1938	1947	rBV	1868013	2781977	31.96%	3.787%
30	14.833	1973	1980	1999	rBV3	85785	296450	3.41%	0.404%
31	14.998	2004	2008	2012	rVV6	9320	19581	0.22%	0.027%
32	15.039	2012	2015	2021	rVB8	11147	15889	0.18%	0.022%
33	15.580	2100	2107	2120	rBV	4483290	6619610	76.04%	9.012%
34	15.721	2124	2131	2139	rVV	1200407	1742600	20.02%	2.372%
35	15.798	2139	2144	2155	rVB2	98081	200920	2.31%	0.274%
36	16.368	2235	2241	2246	rBV4	15034	22364	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043867.D
 Acq On : 17 Jan 2024 15:11
 Operator : MA/JU
 Sample : P1142-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

37	16.898	2327	2331	2335	rBV5	6632	10931	0.13%	0.015%
38	17.339	2399	2406	2416	rBV	2402053	3363330	38.64%	4.579%
39	17.439	2416	2423	2440	rVV	5178741	7353259	84.47%	10.011%
40	17.557	2440	2443	2451	rVB9	12496	26069	0.30%	0.035%
41	18.074	2526	2531	2537	rBV8	19829	31042	0.36%	0.042%
42	18.239	2554	2559	2568	rBV4	41564	71926	0.83%	0.098%
43	18.668	2629	2632	2635	rBV5	7463	10468	0.12%	0.014%
44	18.862	2661	2665	2670	rVB6	15737	23509	0.27%	0.032%
45	19.162	2713	2716	2717	rBV3	10159	10642	0.12%	0.014%
46	19.298	2735	2739	2745	rBV	58139	77928	0.90%	0.106%
47	19.368	2747	2751	2755	rBV	46885	64890	0.75%	0.088%
48	19.515	2773	2776	2781	rBV7	15351	28385	0.33%	0.039%
49	19.668	2799	2802	2806	rVB3	19581	21080	0.24%	0.029%
50	19.733	2807	2813	2826	rVV	6472743	8549821	98.21%	11.639%
51	21.527	3113	3118	3130	rBV	2559012	3610892	41.48%	4.916%
52	23.791	3496	3503	3511	rBV2	4396936	8705345	100.00%	11.851%
53	23.950	3523	3530	3547	rVB	1803927	3817825	43.86%	5.197%




Sum of corrected areas: 73455418

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043867.D
Acq On : 17 Jan 2024 15:11
Operator : MA/JU
Sample : P1142-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

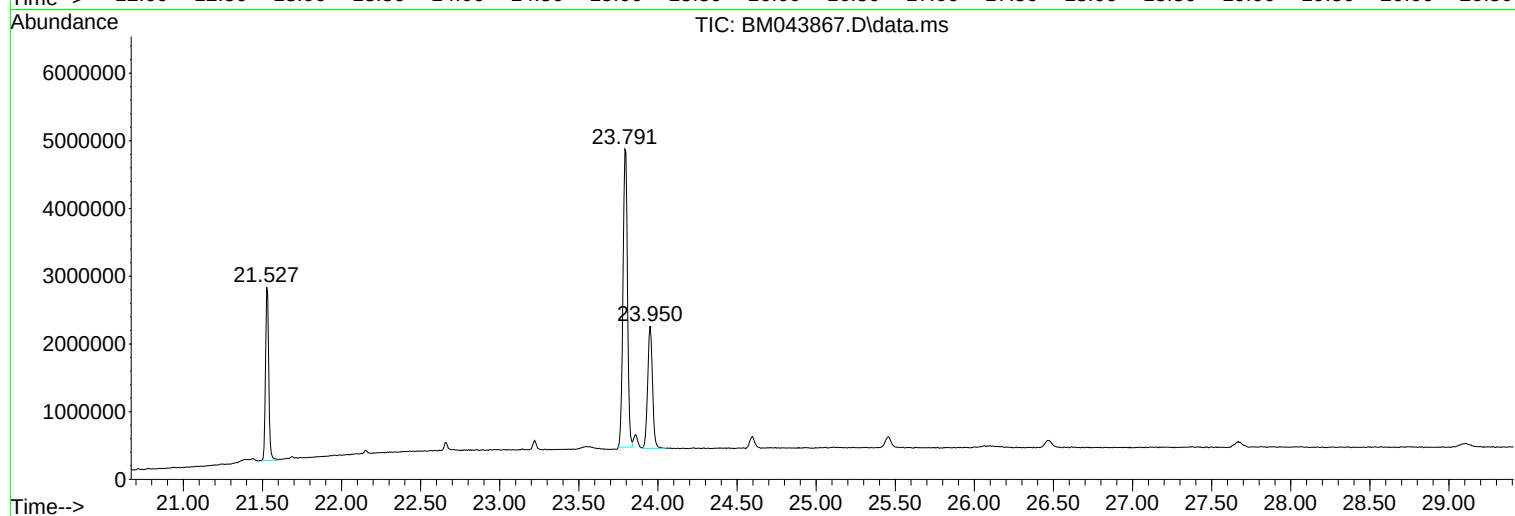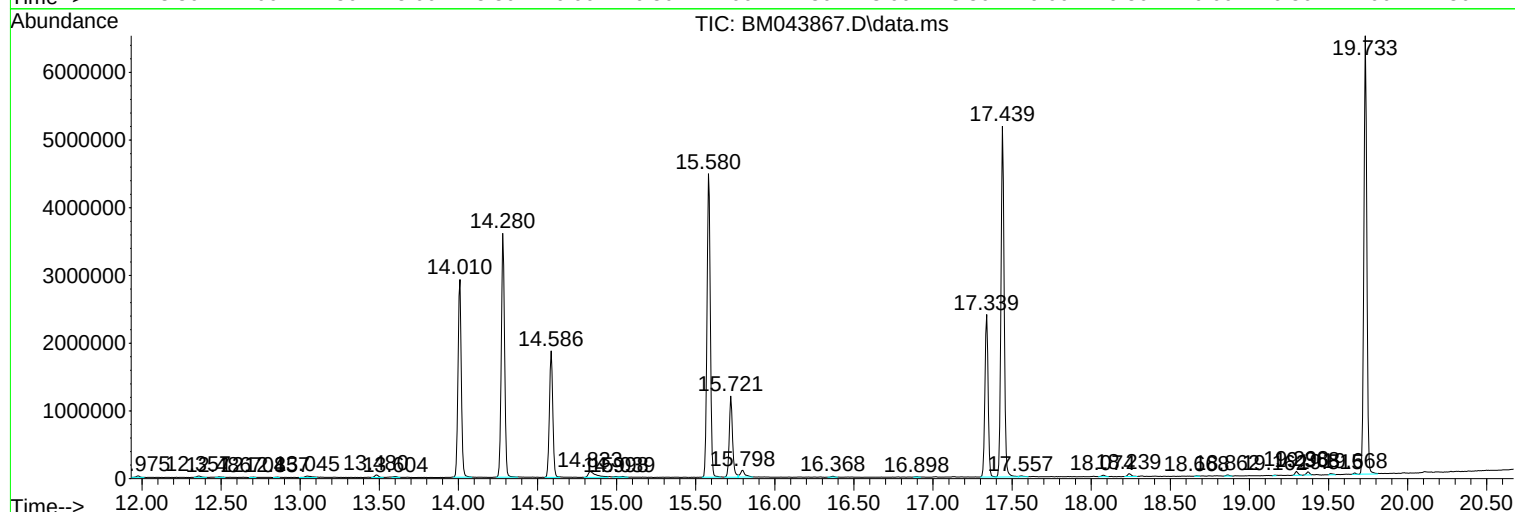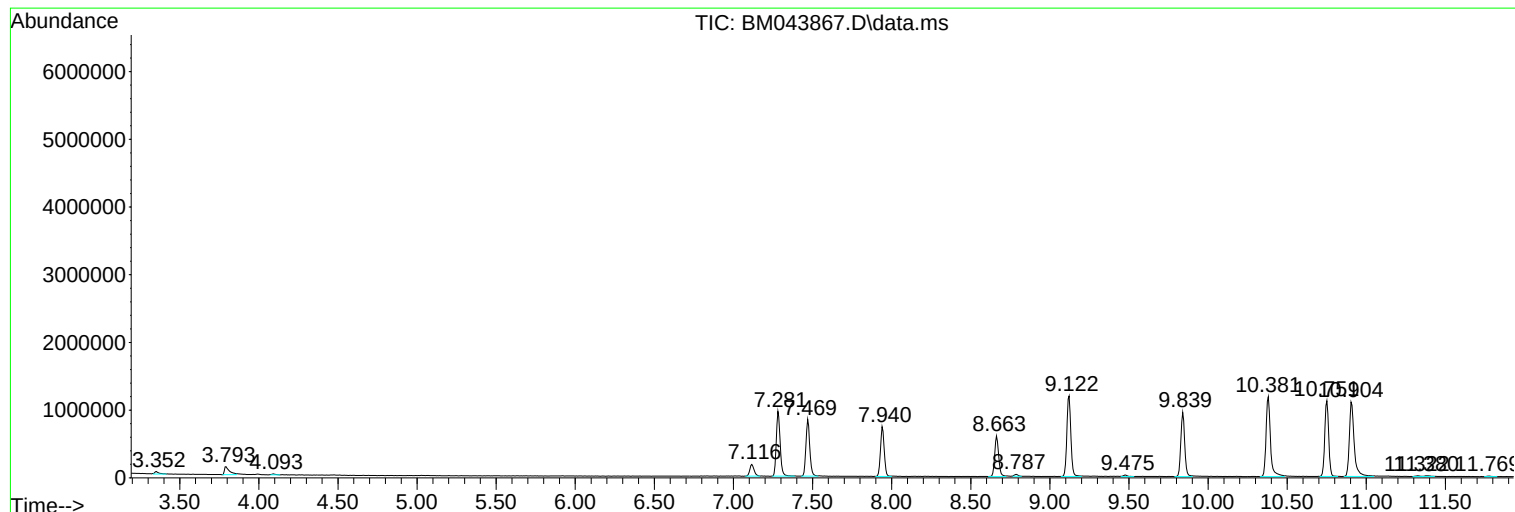

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043867.D
Acq On : 17 Jan 2024 15:11
Operator : MA/JU
Sample : P1142-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043867.D
Acq On : 17 Jan 2024 15:11
Operator : MA/JU
Sample : P1142-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc