

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043868.D
 Acq On : 17 Jan 2024 15:48
 Operator : MA/JU
 Sample : P1142-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	34	rBV	44912	66336	0.65%	0.087%
2	3.793	99	103	115	rBV	112380	249189	2.43%	0.325%
3	4.093	151	154	159	rVB2	15490	21758	0.21%	0.028%
4	5.052	314	317	331	rVB	36341	63831	0.62%	0.083%
5	7.116	661	668	682	rVB	200244	370301	3.61%	0.483%
6	7.281	688	696	709	rBV	1011292	1649879	16.09%	2.151%
7	7.469	721	728	742	rBV	860934	1442130	14.06%	1.881%
8	7.940	801	808	816	rBV	823676	1346799	13.13%	1.756%
9	8.010	818	820	826	rVB4	6544	10450	0.10%	0.014%
10	8.663	923	931	943	rBV	630318	1097478	10.70%	1.431%
11	8.787	948	952	960	rVB2	24179	47726	0.47%	0.062%
12	9.122	1001	1009	1022	rBV	1194728	2070095	20.18%	2.699%
13	9.839	1121	1131	1143	rBV	633723	1087315	10.60%	1.418%
14	10.381	1215	1223	1246	rBV	1115272	2147027	20.93%	2.800%
15	10.751	1278	1286	1293	rBV	1217877	2044754	19.94%	2.666%
16	10.904	1305	1312	1333	rBV	995362	2148231	20.94%	2.801%
17	11.322	1380	1383	1389	rBV5	7439	13082	0.13%	0.017%
18	11.386	1390	1394	1398	rVV5	7393	10780	0.11%	0.014%
19	11.775	1455	1460	1465	rBV4	7765	12775	0.12%	0.017%
20	12.357	1554	1559	1566	rVB	20865	37568	0.37%	0.049%
21	12.451	1568	1575	1577	rBV6	5491	13237	0.13%	0.017%
22	12.486	1579	1581	1587	rVB7	7695	12911	0.13%	0.017%
23	13.039	1668	1675	1689	rBV2	36112	107465	1.05%	0.140%
24	13.439	1739	1743	1746	rBV	9552	13571	0.13%	0.018%
25	13.480	1746	1750	1757	rVV	34089	57397	0.56%	0.075%
26	13.598	1767	1770	1774	rVB3	11661	16701	0.16%	0.022%
27	13.922	1821	1825	1830	rBV6	6780	11719	0.11%	0.015%
28	14.010	1833	1840	1850	rBV	3023340	4285895	41.79%	5.589%
29	14.280	1878	1886	1900	rBV	3506760	5127559	49.99%	6.686%
30	14.586	1931	1938	1948	rBV	1949535	2898734	28.26%	3.780%
31	14.833	1974	1980	1996	rBV	84954	267661	2.61%	0.349%
32	15.580	2100	2107	2123	rBV	4593102	6679173	65.12%	8.710%
33	15.721	2123	2131	2139	rBV	751547	1172260	11.43%	1.529%
34	15.798	2139	2144	2153	rVB2	91395	174374	1.70%	0.227%
35	16.368	2235	2241	2249	rVB9	14887	27144	0.26%	0.035%
36	17.339	2397	2406	2416	rBV	2591636	3496610	34.09%	4.560%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
 Data File : BM043868.D
 Acq On : 17 Jan 2024 15:48
 Operator : MA/JU
 Sample : P1142-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

37	17.439	2416	2423	2440	rVV	5802329	8161109	79.57%	10.642%
38	17.557	2440	2443	2449	rVB7	8576	17397	0.17%	0.023%
39	18.015	2515	2521	2525	rBV8	10322	16439	0.16%	0.021%
40	18.074	2527	2531	2538	rVB6	19799	32526	0.32%	0.042%
41	18.239	2554	2559	2566	rBV6	39631	68297	0.67%	0.089%
42	18.862	2660	2665	2671	rBV7	15783	26774	0.26%	0.035%
43	19.298	2734	2739	2746	rBV3	63073	100395	0.98%	0.131%
44	19.368	2747	2751	2757	rBV	50619	71195	0.69%	0.093%
45	19.515	2773	2776	2781	rBV7	14865	23220	0.23%	0.030%
46	19.662	2798	2801	2805	rVB4	16018	19944	0.19%	0.026%
47	19.733	2807	2813	2826	rVV	7400078	9610469	93.70%	12.532%
48	21.527	3113	3118	3131	rBV	2838379	3822649	37.27%	4.985%
49	23.797	3496	3504	3511	rBV	5431070	10256803	100.00%	13.375%
50	23.950	3523	3530	3546	rVB	1943386	4159656	40.56%	5.424%




Sum of corrected areas: 76686788

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043868.D
Acq On : 17 Jan 2024 15:48
Operator : MA/JU
Sample : P1142-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

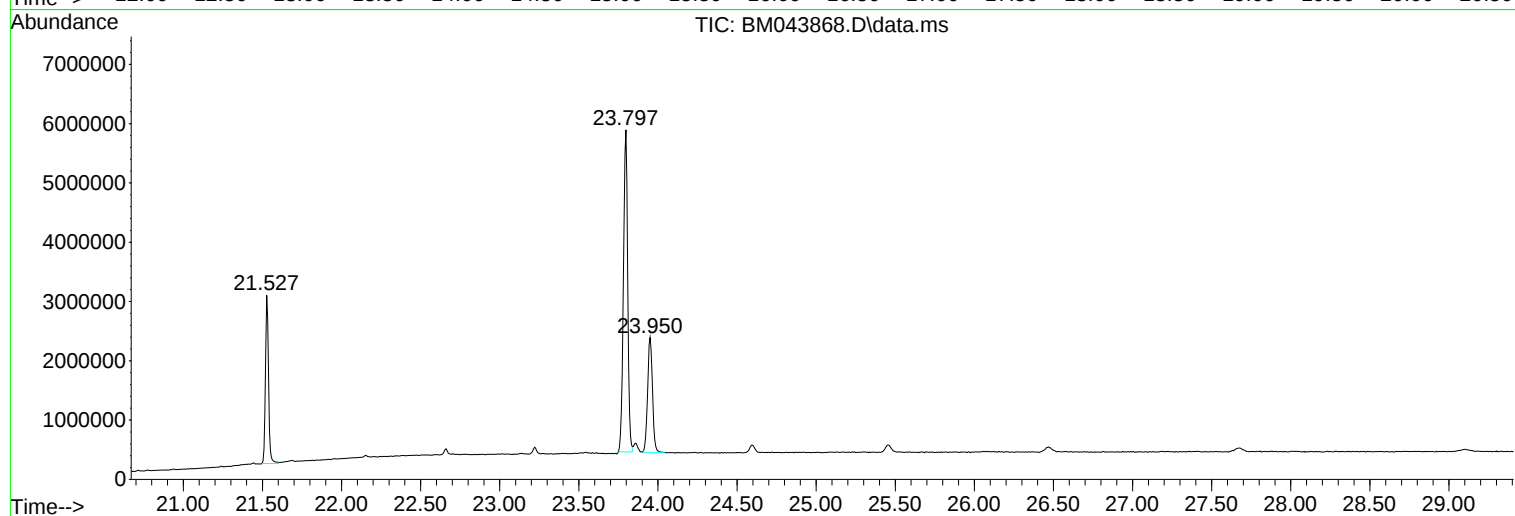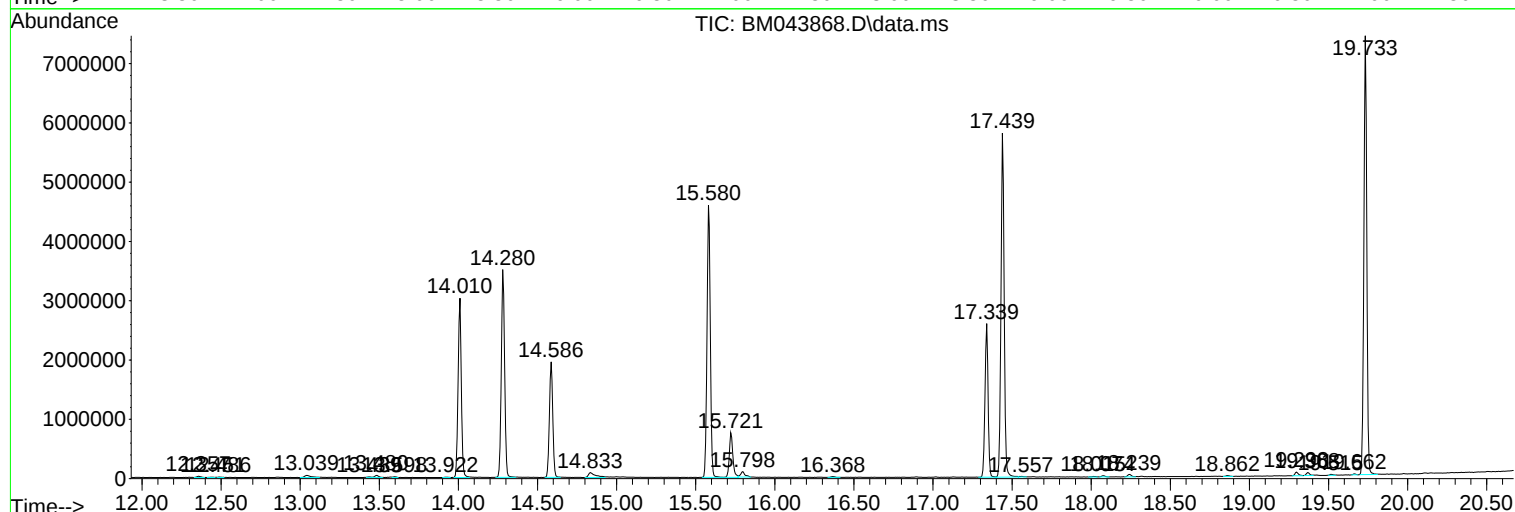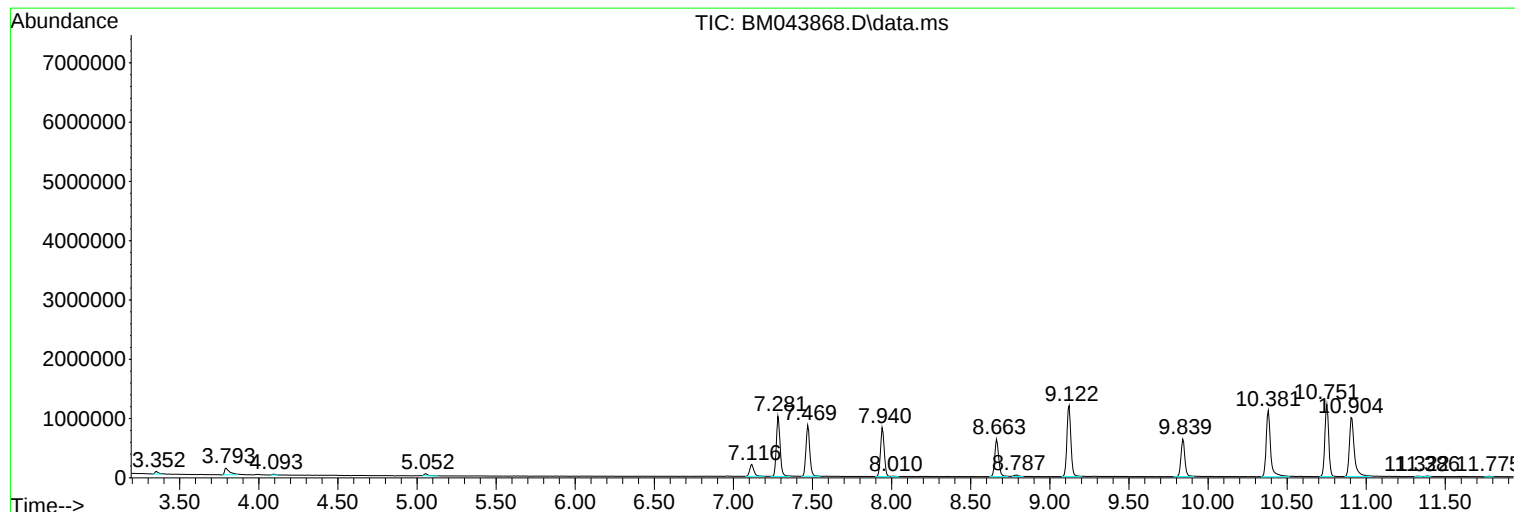

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043868.D
Acq On : 17 Jan 2024 15:48
Operator : MA/JU
Sample : P1142-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011724\
Data File : BM043868.D
Acq On : 17 Jan 2024 15:48
Operator : MA/JU
Sample : P1142-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------