
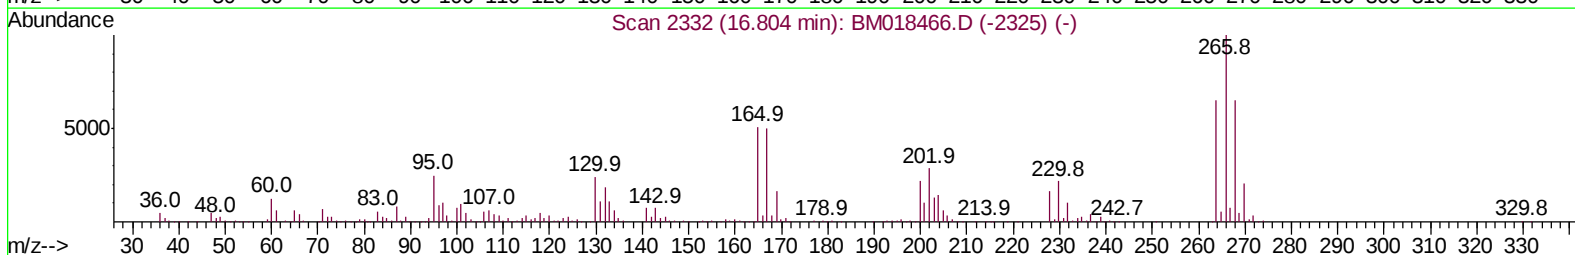
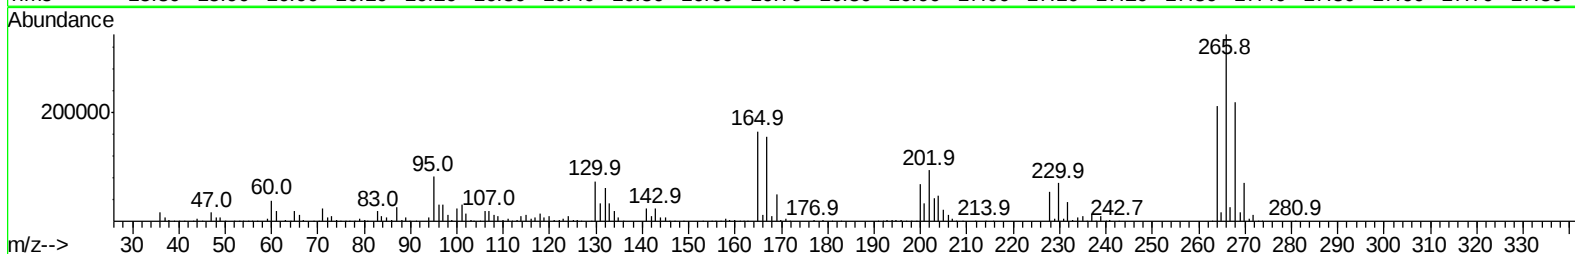


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011819\
Data File : BM018634.D
Acq On : 18 Jan 2019 11:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 22:34:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

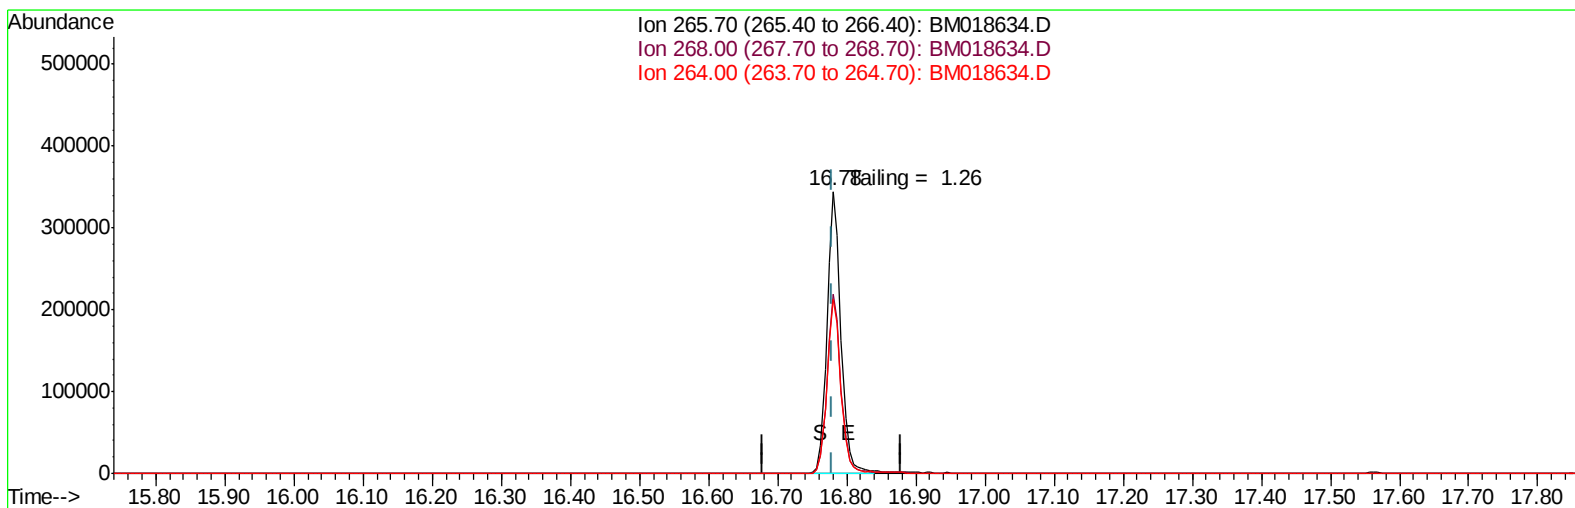

TIC: BM018634.D

(70) Pentachlorophenol (C)




16.780min (+0.000) 58225.71ng

response 480589

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.55
264.00	62.60	61.93
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011819\
Data File : BM018634.D
Acq On : 18 Jan 2019 11:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 22:34:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

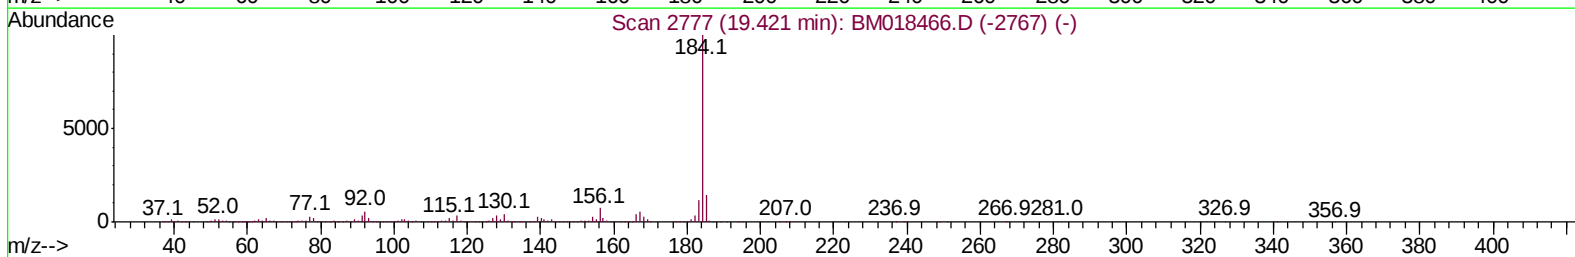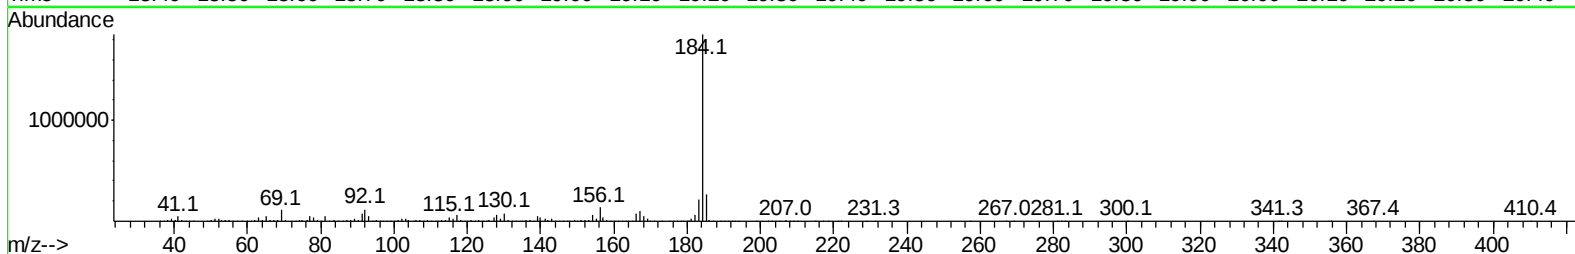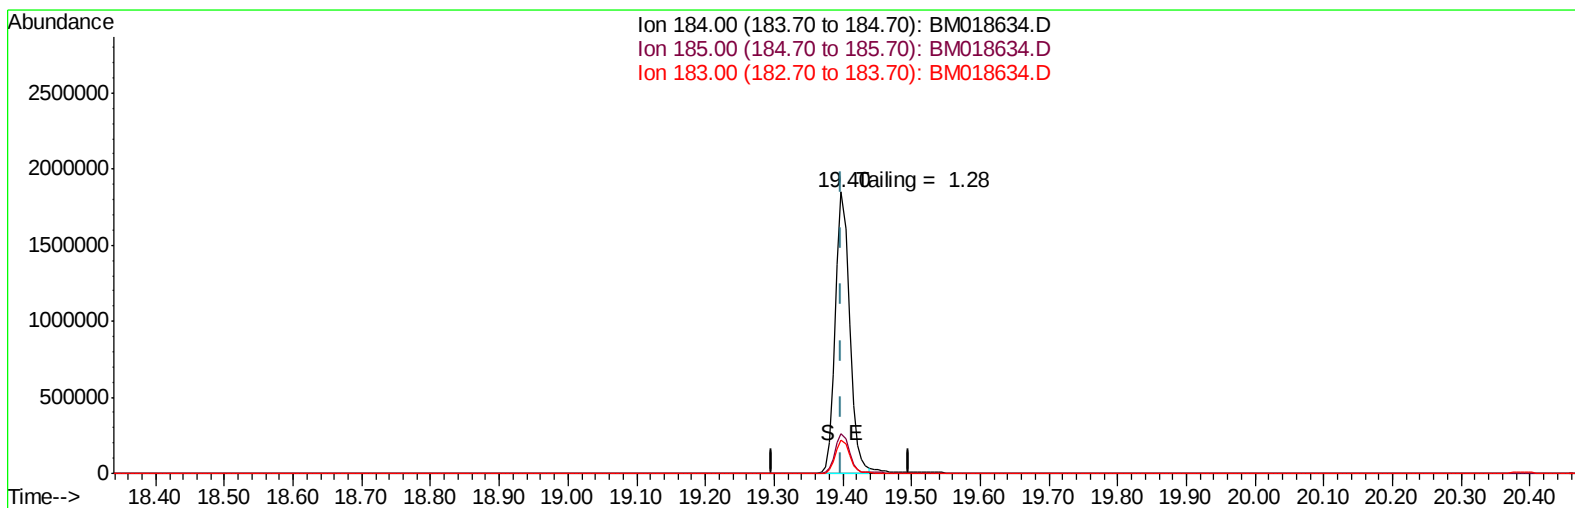

TIC: BM018634.D

(77) Benzidine

19.398min (+0.000) 109290.61ng

response 2685052

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.09
183.00	11.90	12.02
0.00	0.00	0.00