
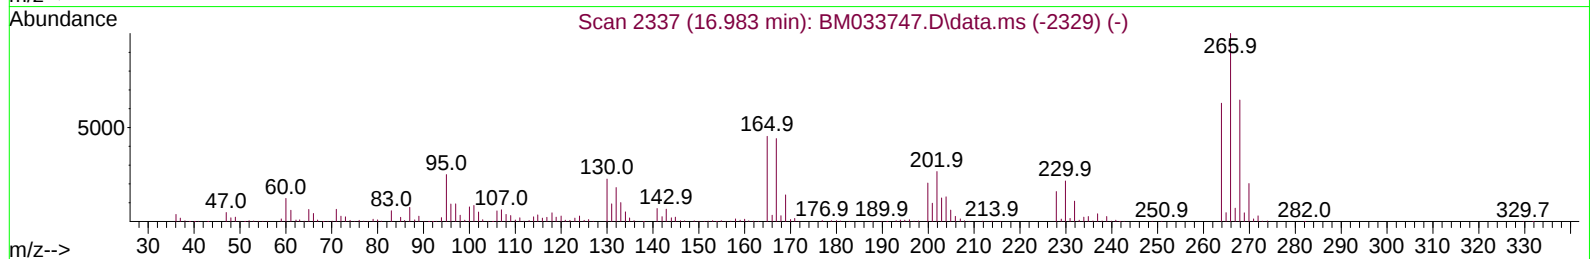
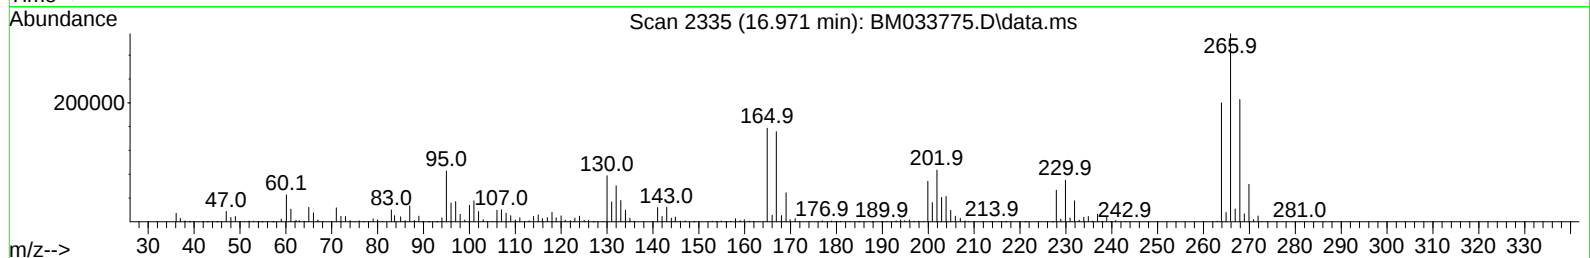


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011922\
Data File : BM033775.D
Acq On : 19 Jan 2022 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 17:38:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 17 16:30:56 2022
Response via : Initial Calibration

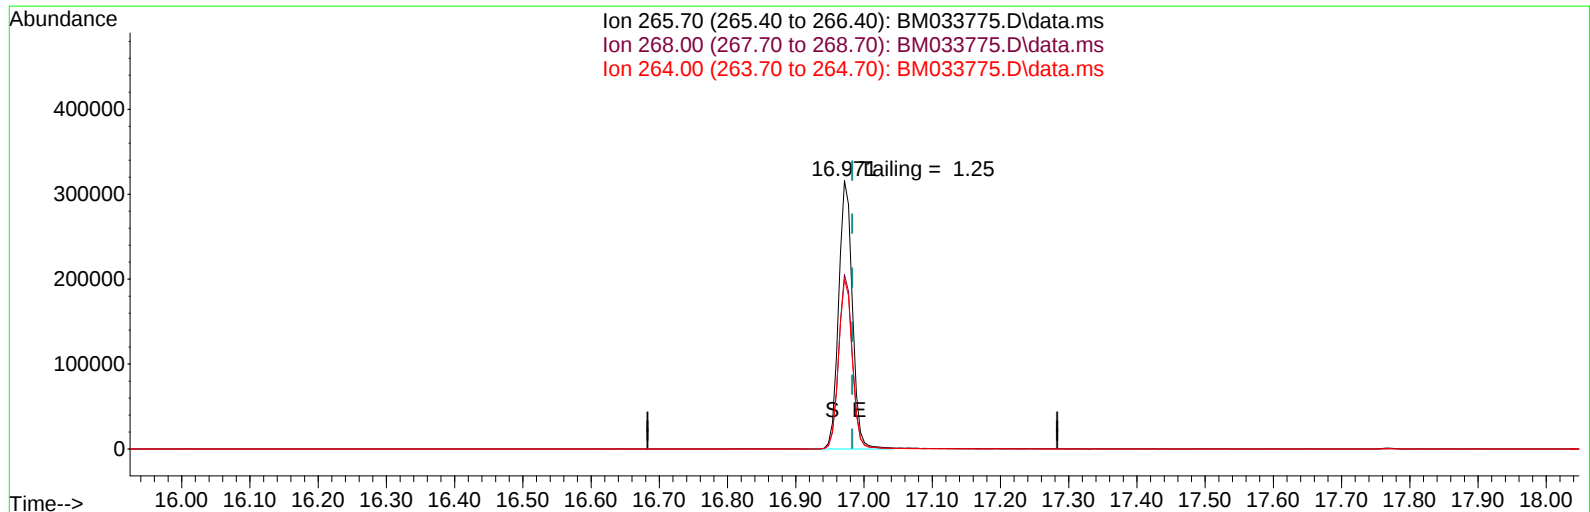

TIC: BM033775.D\data.ms

(70) Pentachlorophenol (C)




16.971min (-0.012) 156917.78 ng

response 444064

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.02
264.00	61.40	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011922\
Data File : BM033775.D
Acq On : 19 Jan 2022 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 17:38:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 17 16:30:56 2022
Response via : Initial Calibration

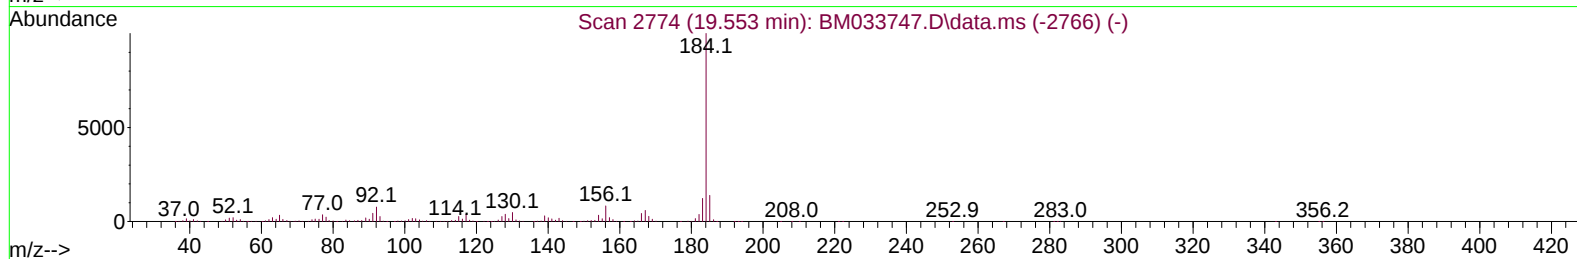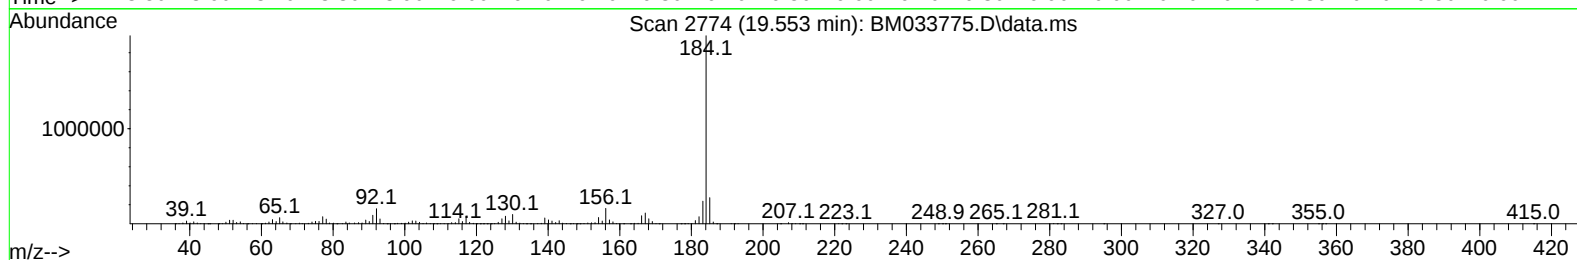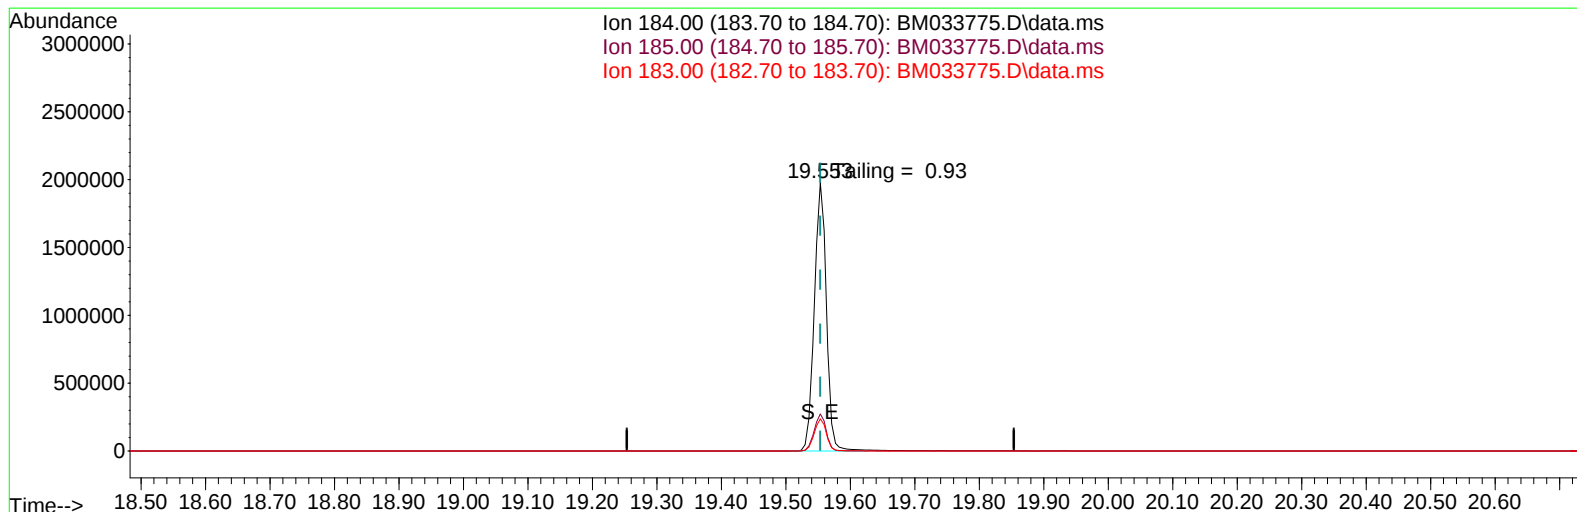

TIC: BM033775.D\data.ms

(77) Benzidine**19.553min (+ 0.000) 12455.07 ng****response 2605424**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.84
183.00	12.10	11.99
0.00	0.00	0.00